




US 20040254476A1

(19) **United States**(12) **Patent Application Publication** (10) **Pub. No.: US 2004/0254476 A1**  
(43) **Pub. Date: Dec. 16, 2004**(54) **LASER DIGITIZER SYSTEM FOR DENTAL APPLICATIONS****Publication Classification**(76) Inventors: **Henley Quadling**, Addison, TX (US);  
**Mark Quadling**, Plano, TX (US); **Alan Blair**, St. Paul, MN (US)(51) **Int. Cl.<sup>7</sup>** ..... **A61B 6/00; G01B 11/24**(52) **U.S. Cl.** ..... **600/476; 356/601**Correspondence Address:  
**BRINKS HOFER GILSON & LIONE**  
**P.O. BOX 10395**  
**CHICAGO, IL 60610 (US)**(57) **ABSTRACT**(21) Appl. No.: **10/804,694**(22) Filed: **Mar. 19, 2004****Related U.S. Application Data**

(60) Provisional application No. 60/457,025, filed on Mar. 24, 2003.

A intra-oral laser digitizer system provides a three-dimensional visual image of a real-world object such as a dental item through a laser digitization. The laser digitizer captures an image of the object by scanning multiple portions of the object in an exposure period. The intra-oral digitizer may be inserted into an oral cavity (in vivo) to capture an image of a dental item such as a tooth, multiple teeth or dentition. The captured image is processed to generate the three-dimension visual image.

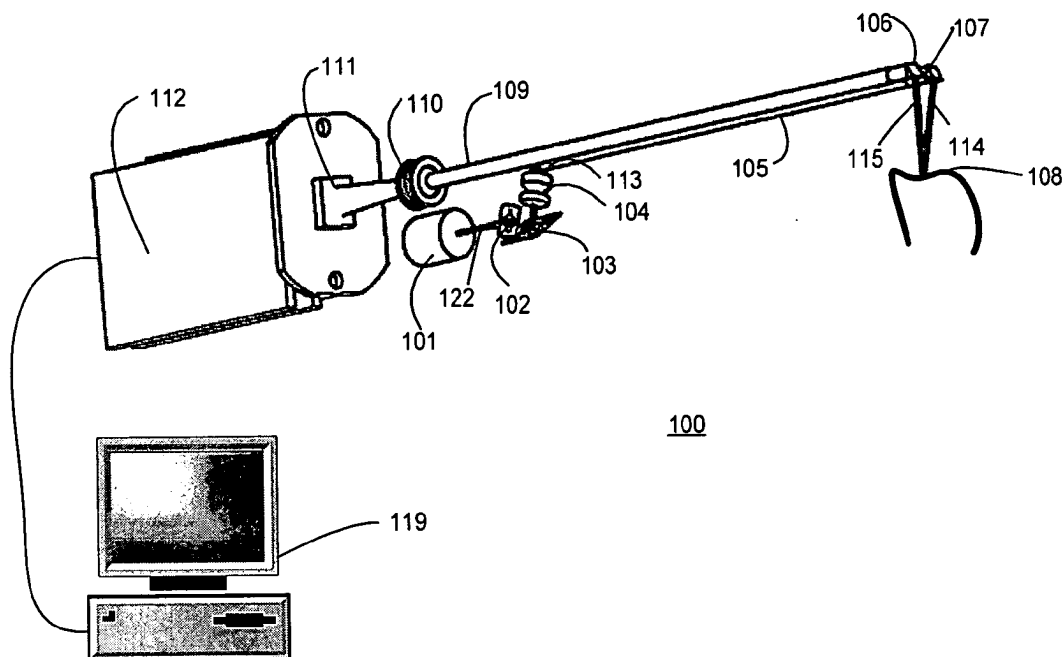100

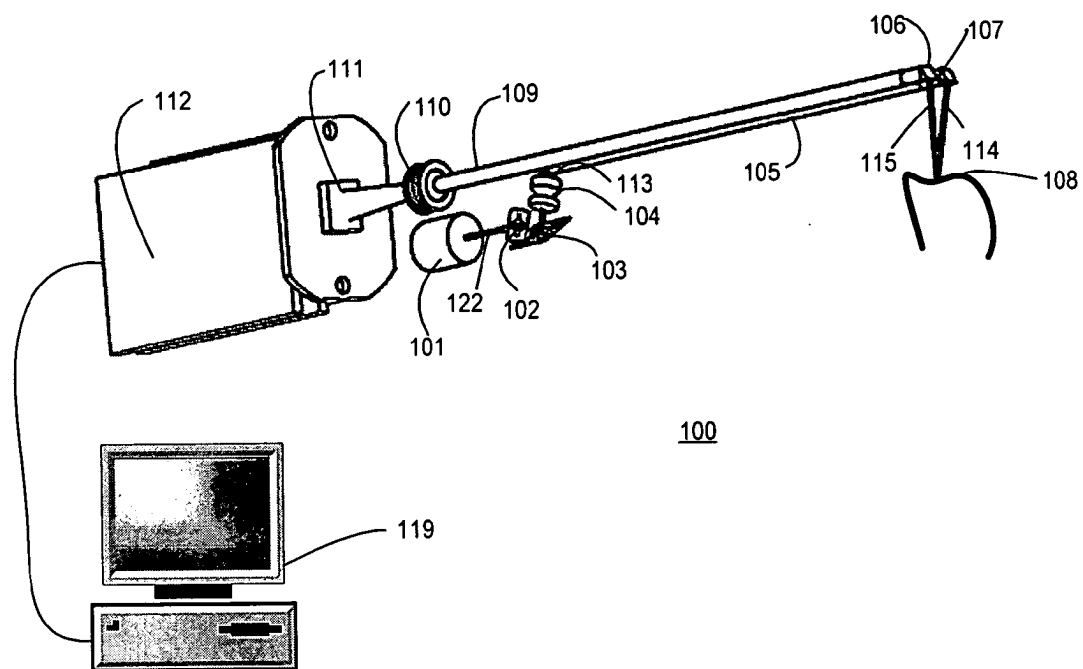
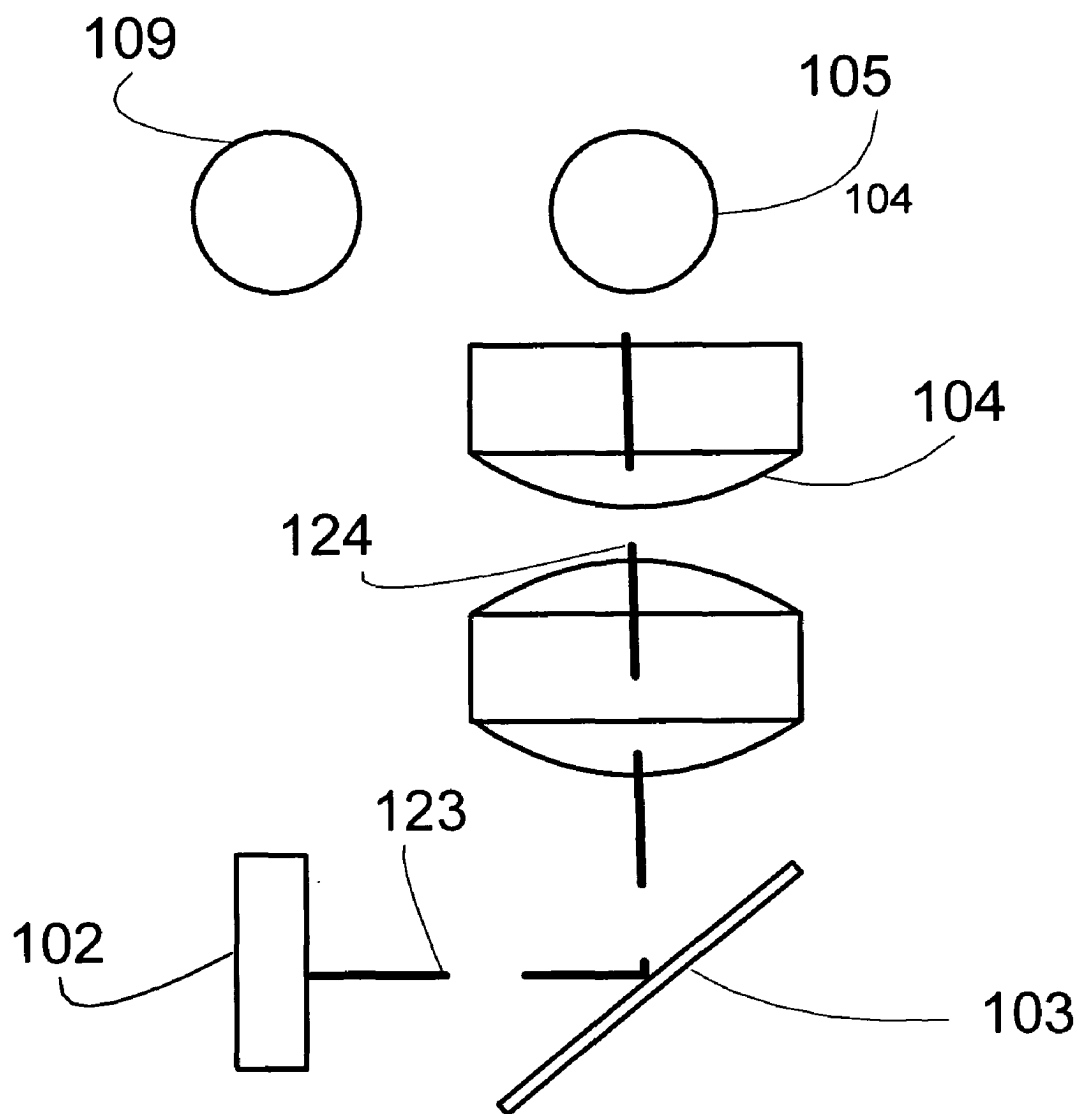


Figure 1



**Figure 2**

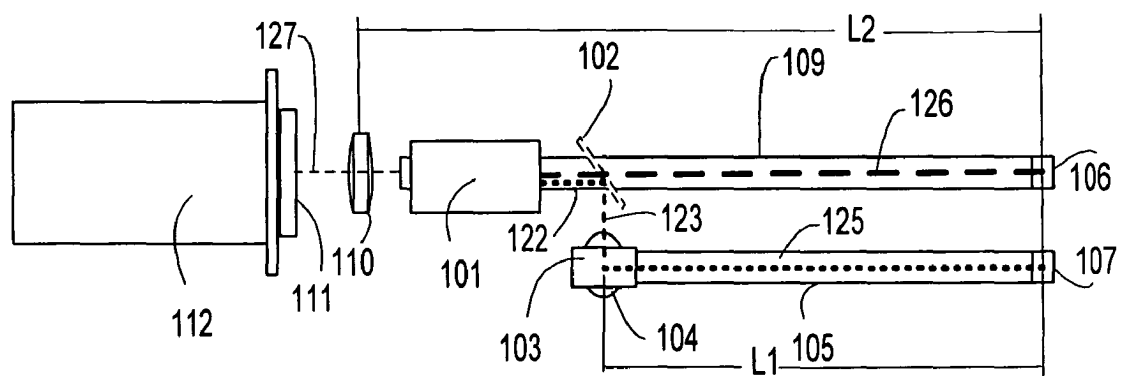


Figure 3

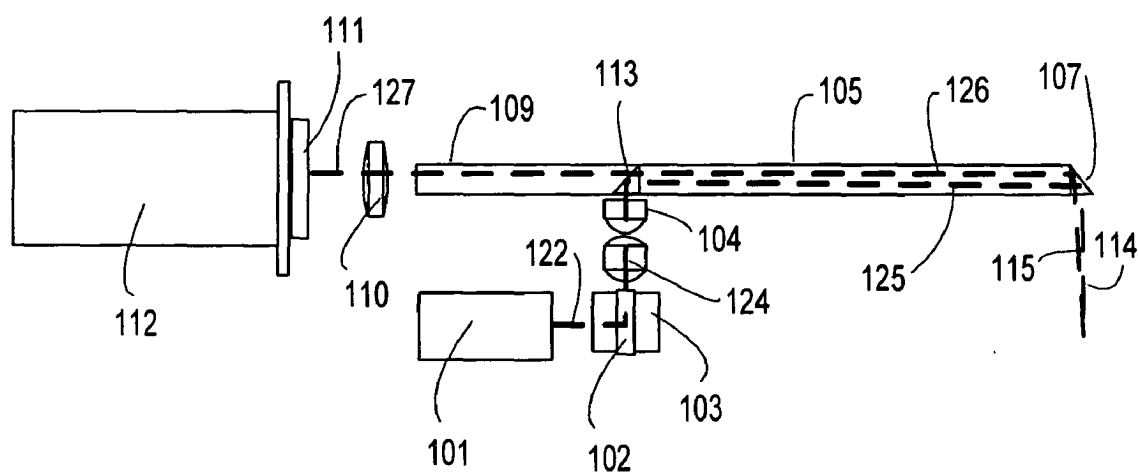
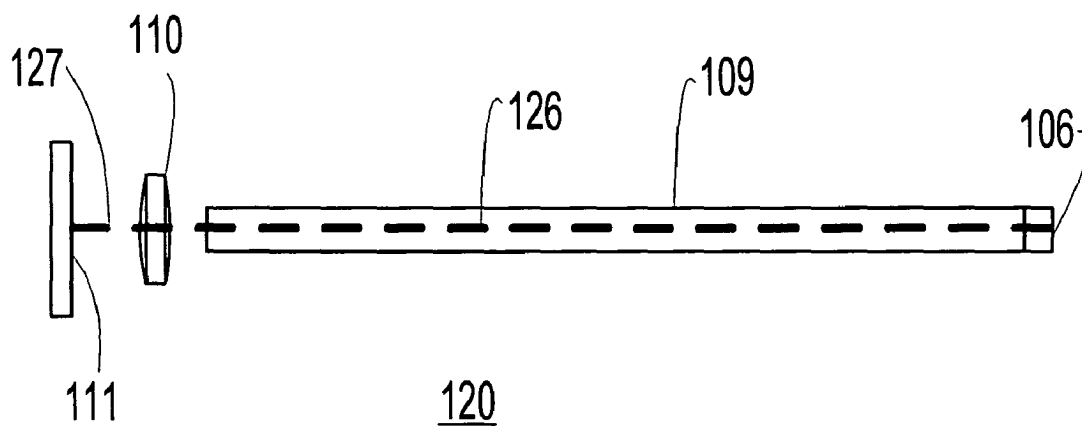
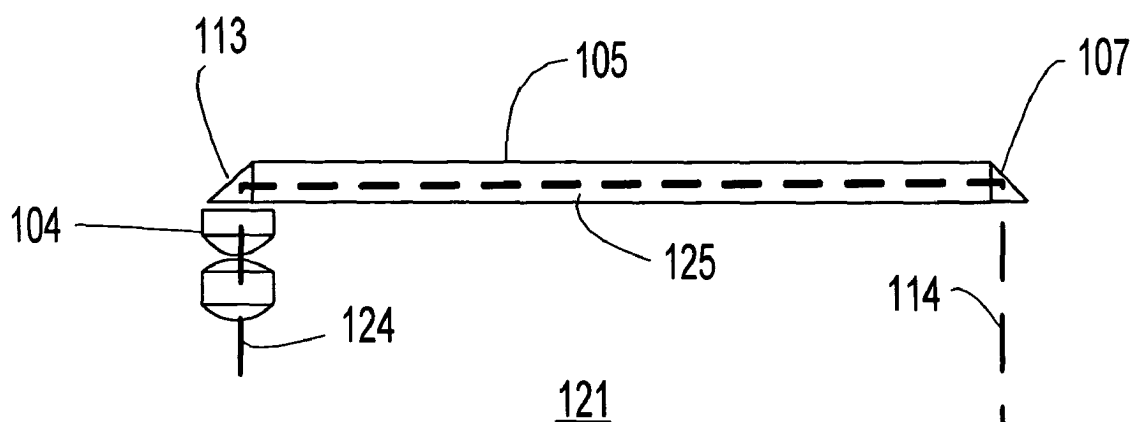


Figure 4



**Figure 5**



**Figure 6**

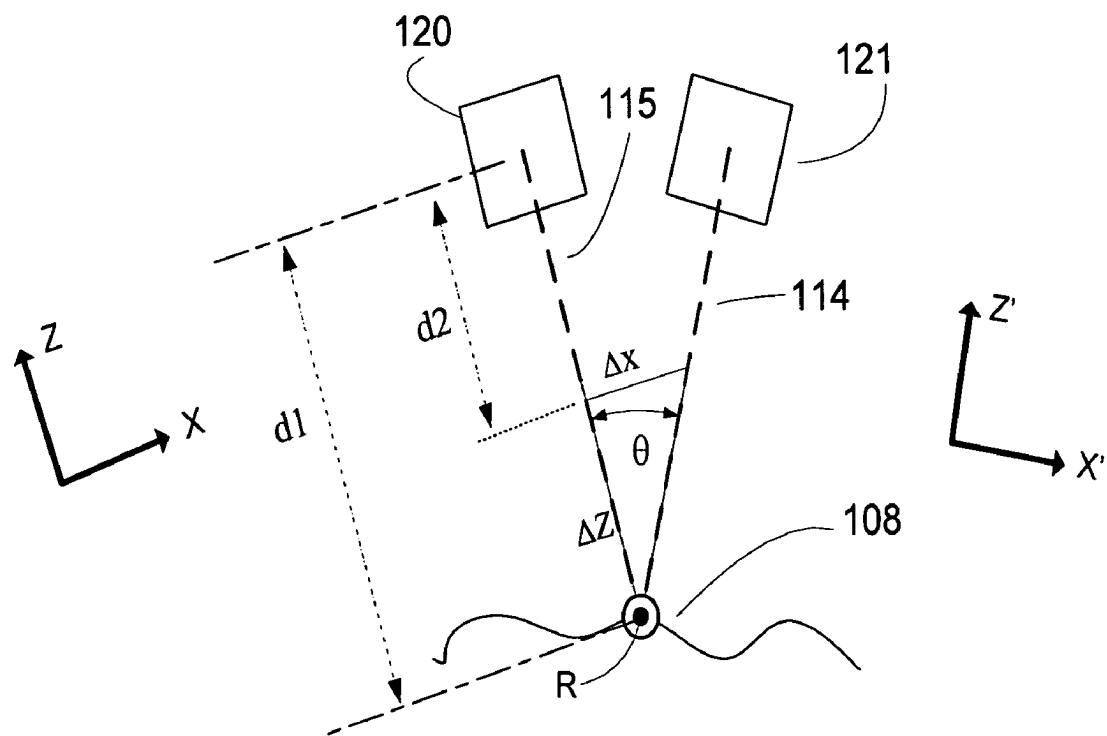


Figure 7



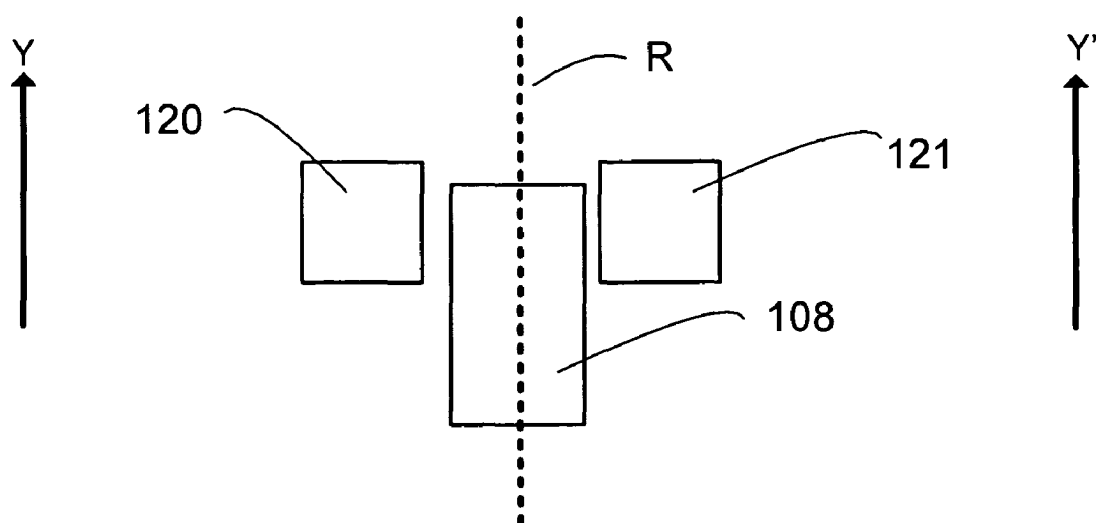
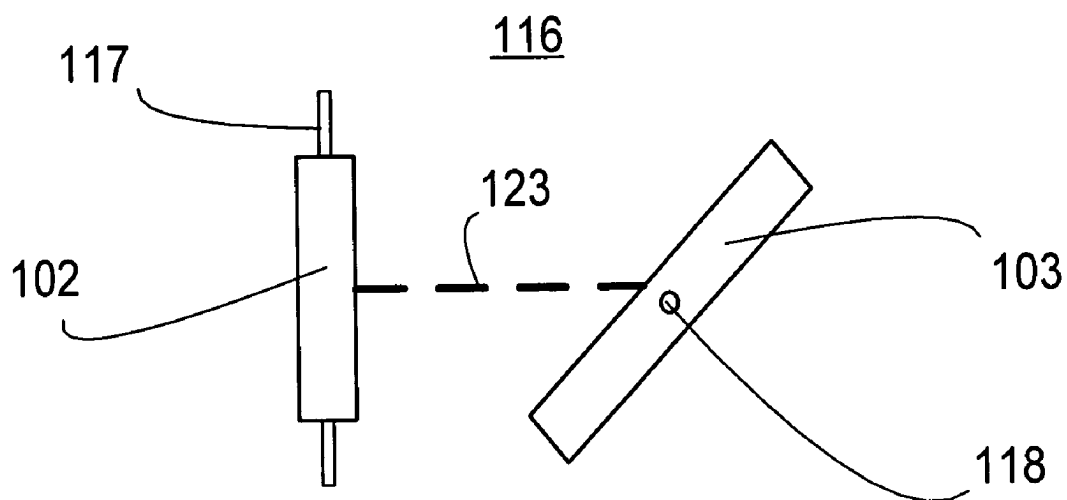


Figure 8



**Figure 9**

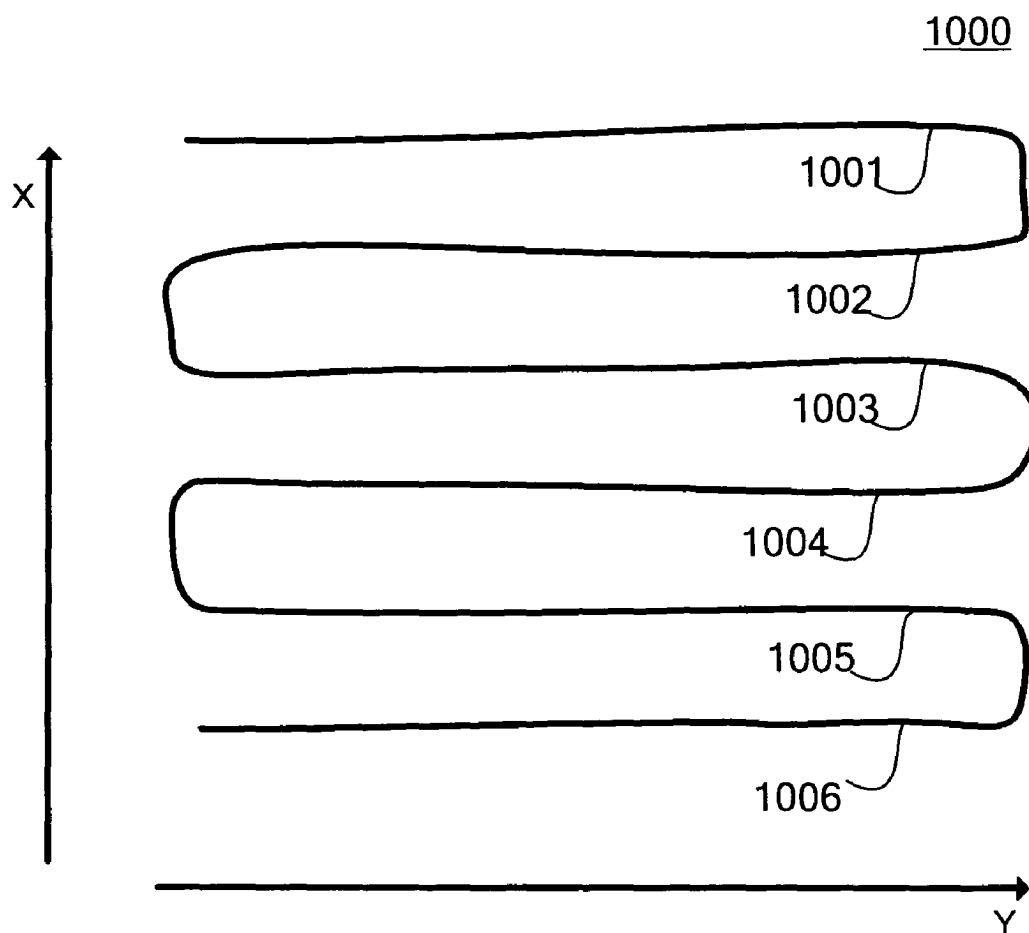


Figure 10

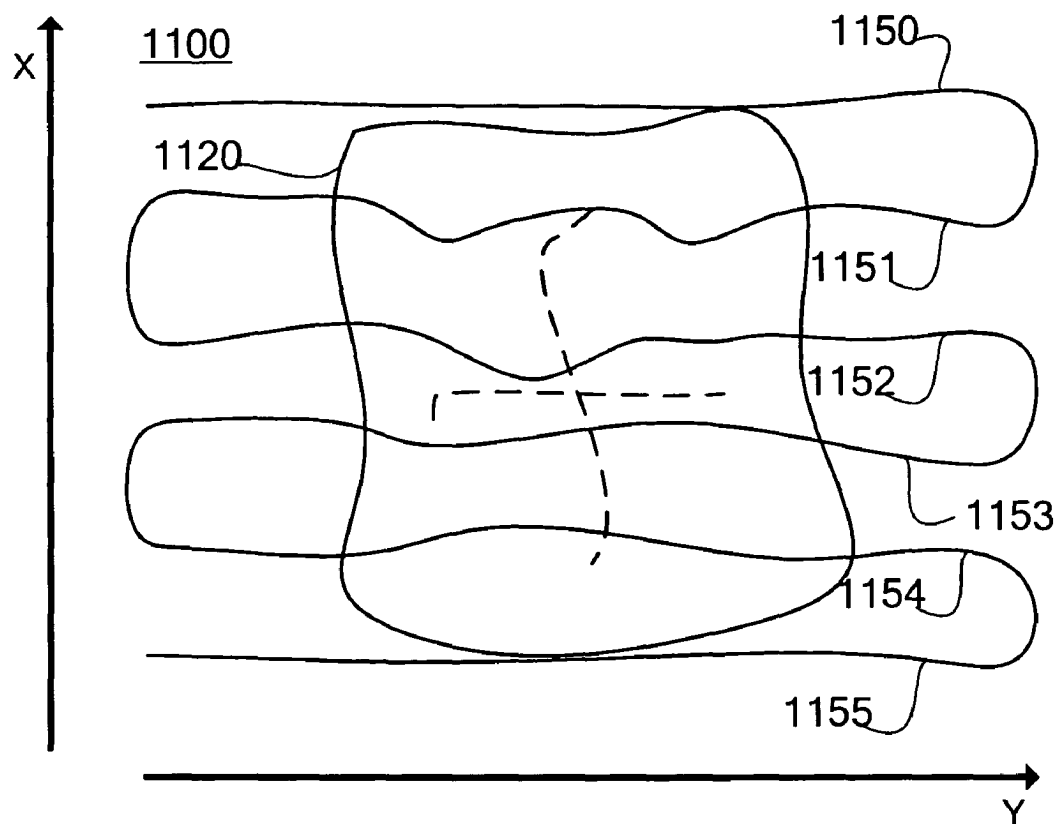


Figure 11

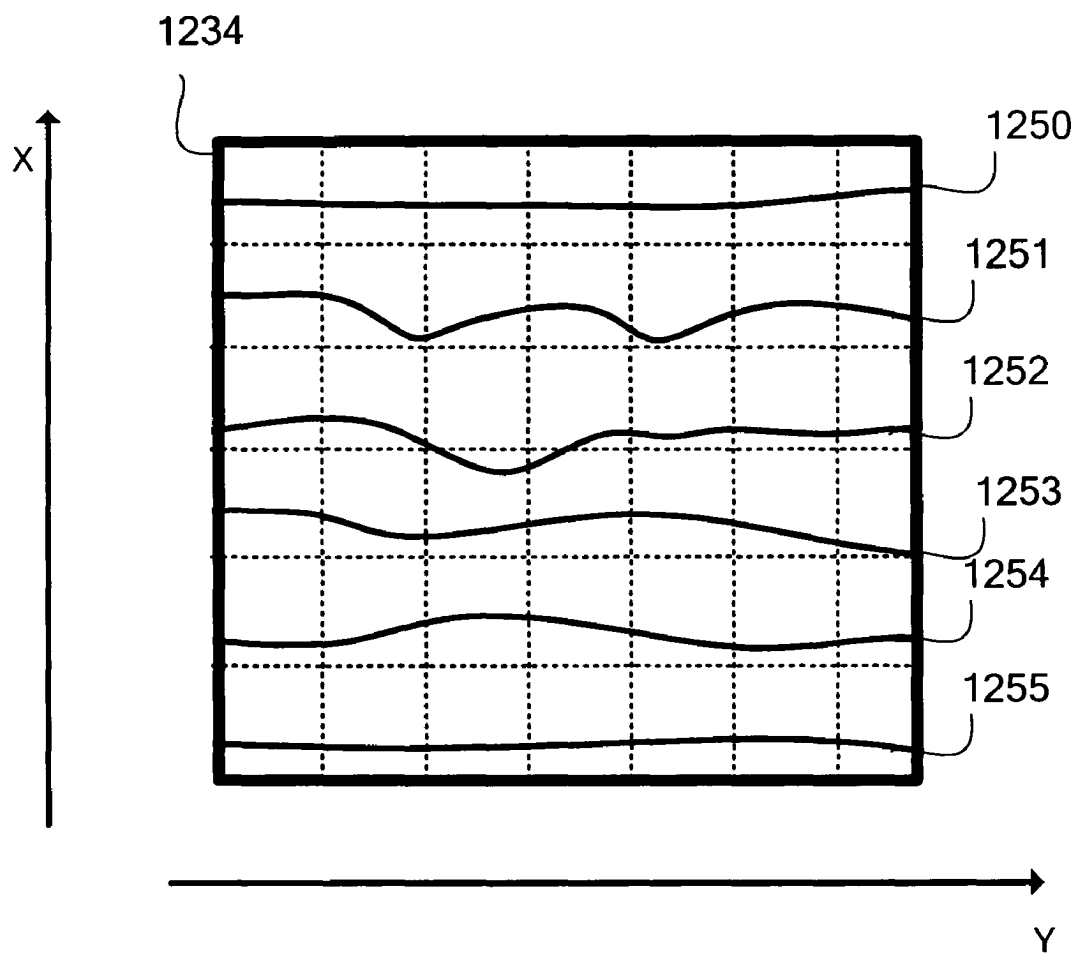


Figure 12

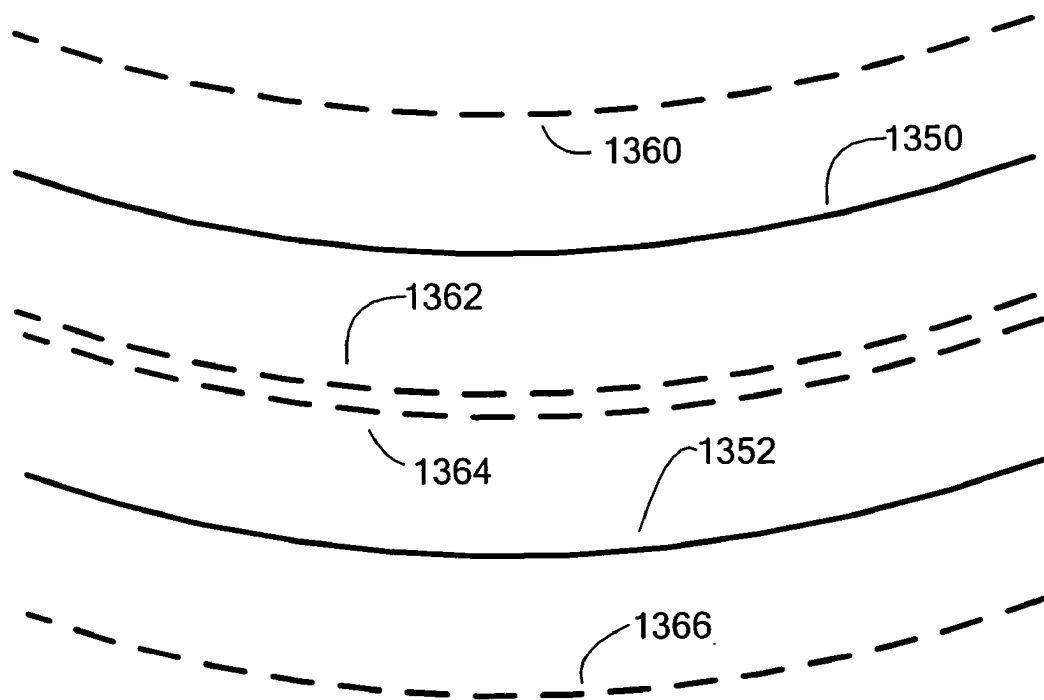


Figure 13


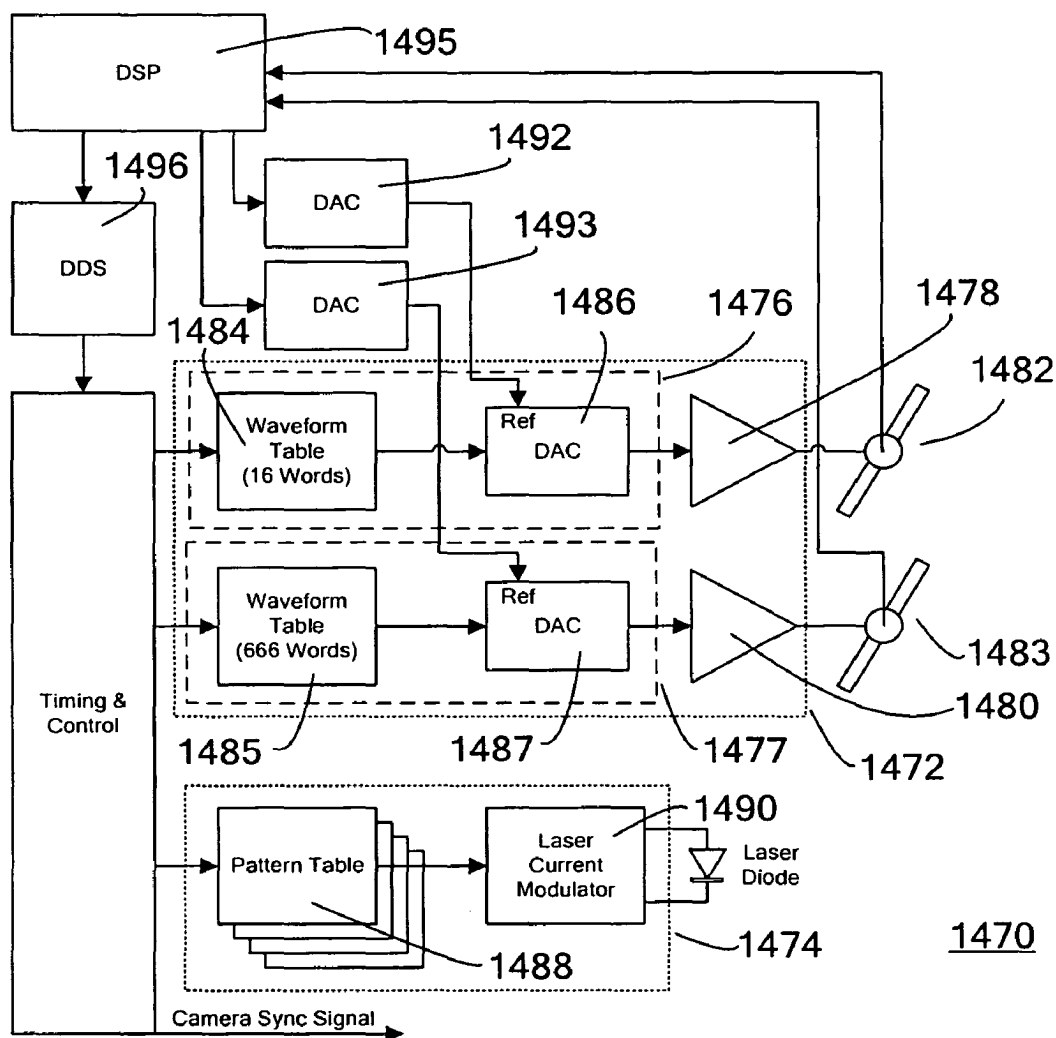


Figure 14



**Figure 15**

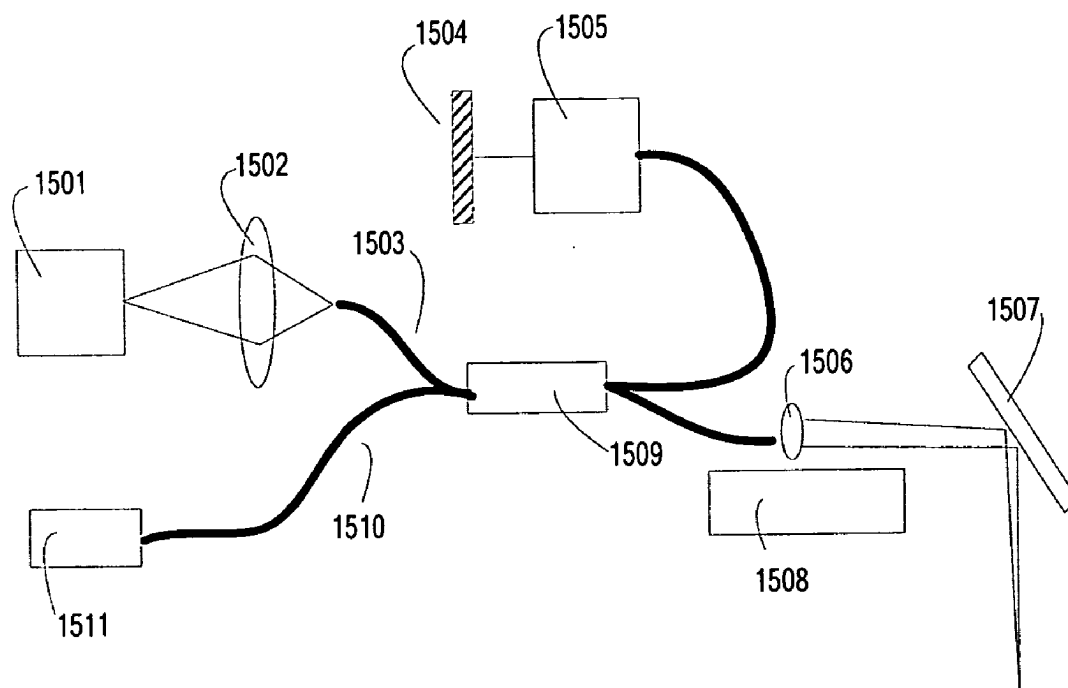

## LASER DIGITIZER SYSTEM FOR DENTAL APPLICATIONS

### PRIORITY AND CROSS REFERENCE TO RELATED APPLICATION

[0001] This application claims the benefit under 35 U.S.C. § 119(e) of co-pending provisional application no. 60/457,025 for Intra-Oral Laser Digitizer System For Dental Applications, which is incorporated in its entirety herein by reference.

### BACKGROUND OF THE INVENTION

#### [0002] 1. Related Field

[0003] The invention relates to three-dimensional imaging of physical objects. In particular, the invention relates to intra-oral (in vivo) laser imaging of dental items including dentition, prepared dentition, impression materials and the like.

#### [0004] 2. Description of the Related Art

[0005] A three-dimensional ("3D") visual image of a physical object may be generated by a computer that processes data representing shapes, surfaces, contours and/or characteristics of the object. The data is generated by optically scanning the object and detecting or capturing the light reflected from the object. Principles such as Moiré, interferometry, and laser triangulation, may be used to model the shape, surfaces, contours and/or characteristics of the object. The computer displays the 3D image on a screen, or computer monitor.

[0006] Existing intra-oral 3D imaging systems use a variation of the Moiré imaging technique. Such systems use structured white light to project a two-dimensional ("2D") depiction on the object to be imaged. Moiré systems use the 2D lateral information, and input from skilled operators, to determine relative dimensions of adjacent features. Moiré systems also use a sinusoidal intensity pattern that is observed from a position other than a projection angle that does not appear sinusoidal. Therefore, an inferred point-by-point phase angle between an observed and a projected image may be correlated to height data.

[0007] Intra-oral dental imaging systems, based on the Moiré technique image a dental item, such as a tooth, directly from or below occlusal surfaces of the tooth. Such systems have low depth resolution and may not accurately image or represent a surface that is undercut or shadowed. Intra-oral dental imaging systems also may require a powder or the like to provide a uniform color and reflectivity required by limitations of the white light techniques. The powder layer may increase or introduce errors in the digitized data, due to non-uniformity of the powder thickness.

### BRIEF SUMMARY OF THE INVENTION

[0008] The embodiments provide a laser imaging system that generates a three-dimensional image of a scanned physical object such as a dental item. An embodiment includes intra-oral laser imaging systems, methods, apparatuses, and techniques that provide digitization of a physical object to generate a 3D visual image of the object. An intra-oral digitizer generates a laser pattern that may be projected on or towards a dental item, dentition, prepared

dentition, or impression material in an oral cavity (in vivo). The intra-oral digitizer may include a projection optics system that remotely generates the laser pattern and relays that pattern so that it may be projected on or towards a dental item or items in vivo. The intra-oral digitizer also includes an imaging optical system that detects or captures light reflected from the dental item. The imaging optical system, or a portion thereof, may be inserted in the oral cavity at a known angle with respect to the projection system to capture light reflected from the dentition. The captured light may be used to generate data representative of the 3D image of the dentition. The 3D visual image may be displayed on a computer monitor, screen, display, or the like. The data also may be used to form a dental restoration using known techniques such as milling techniques. The restoration may be a crown, bridge, inlay, onlay, implant or the like.

[0009] The intra-oral laser digitizer may have a light source, a focusing objective, a two-axis scanner, an optical relay system, an image optics system, and a processor configured to carry out instructions based on code, and process digital data. The light source may have a laser LED and collimating optics producing a collimated beam of light that is projected to the two-axis scanner. The scanner redirects, or scans, the collimated beam of light through at least two axes at high speeds. The scanner may scan the beam at a selected constant frequency or a variable frequency and duty cycle. The scanned beam is projected toward the optical relay system, which focuses the beam as a dot on the surface of the object.

[0010] The optical relay system may include focusing lenses, relay lenses and a prism, through which the scanned beam may be projected. The optical relay system focuses the desired pattern of the laser dot generated by the scanner on the object. The laser dot may be focused so that the dot traverses a curvilinear segment across the object. The optical relay system may include one or more optical components such as standard optical glass lenses, or gradient index glass lenses.

[0011] The image capture instrument detects the light reflected from the object through a relay optics system. The image capture system generates data representing a captured image of the scanned beam. The image capture system may be configured to capture images of one or more scanned curvilinear segments during an exposure period. The computer processes the data to generate the three-dimensional visual image of the object on a computer monitor, a screen, or other display.

[0012] Multiple images of the object may be recorded and processed by the computer to produce a 3D map of the object. The multiple images can be captured from multiple positions and orientations with respect to the object. The individual images are merged to create an overall 3D map of the object. The images may be captured and processed to provide a real time image of the surface of the object. The real time image may provide an instant feedback mechanism to an operator of the system. The digitizer system may include software that displays the overall 3D image captured in real time. The software also may include feedback and identification provided to the operator of suggested viewpoints to complete the overall 3D image. The software also may identify crucial features in the scanned data set during a data acquisition process. These features include margins

and neighboring dentition. This software also may display highlighted features or possible problem areas, as the operator captures additional viewpoints.

[0013] A one- or two-axis tilt sensor may determine a relative angle between images. The imaging system may also be used as a standard 2D dental camera through the addition of a background light source.

[0014] Control, acquisition, and interaction may be initiated via foot controls, controls on the intra-oral device, or by voice recognition of spoken commands, or like methods.

[0015] An embodiment quickly and accurately digitizes 3D surfaces of an object, such as prepared teeth and impression materials including bite registration strips. The intra-oral digitizer also provides improved imaging abilities over prior art intra-oral dental imaging systems. The digitizer also simplifies operator requirements and interactions for an intra-oral dental scanning system.

[0016] Other systems, methods, features and advantages of the invention will be, or will become, apparent to one with skill in the art upon examination of the following figures and detailed description. It is intended that all such additional systems, methods, features and advantages be included within this description, be within the scope of the invention, and be protected by the following claims.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0017] The invention can be better understood with reference to the following drawings and description. The components in the figures are not necessarily to scale, emphasis instead being placed upon illustrating the principles of the invention. Moreover, in the figures, like referenced numerals designate corresponding parts throughout the different views.

[0018] FIG. 1 illustrates an intra-oral laser digitizer coupled to a processor.

[0019] FIG. 2 illustrates a front view of a portion of the intra-oral laser digitizer of FIG. 1.

[0020] FIG. 3 illustrates a top view of the intra-oral laser digitizer of FIG. 1.

[0021] FIG. 4 illustrates a side view the intra-oral laser digitizer of FIG. 1.

[0022] FIG. 5 illustrates an imaging optical system of the intra-oral laser digitizer of FIG. 1.

[0023] FIG. 6 illustrates a projection optics system of the intra-oral laser digitizer of FIG. 1.

[0024] FIG. 7 illustrates a projection of a laser light beam on an object.

[0025] FIG. 8 illustrates a top view of a projection of a laser light beam.

[0026] FIG. 9 illustrates a two-axis scanner of the intra-oral laser digitizer of FIG. 1.

[0027] FIG. 10 illustrates an image of a light pattern of the intra-oral digitizer, as projected on and viewed from a flat surface.

[0028] FIG. 11 illustrates the light pattern of FIG. 10 as projected on an object to be imaged.

[0029] FIG. 12 illustrates a reflection of the light pattern of FIG. 10 as detected by image capture instrument.

[0030] FIG. 13 illustrates multiple laser profiles projected towards an object.

[0031] FIG. 14 illustrates an electronic circuit that for controlling the generation of a line pattern.

[0032] FIG. 15 illustrates an intra-oral digitizer with a low coherence light source coupled to the scanning system and a coupler to a reference beam on an optical delay line.

#### DESCRIPTION OF THE EMBODIMENTS OF THE INVENTION

[0033] FIG. 1 illustrates an example of an intra-oral laser digitizer 100. FIGS. 2-5 illustrate various views of the intra-oral laser digitizer 100 of FIG. 1. The intra-oral digitizer 100 generates a 3D image of an object 108 such as a dental item. The intra-oral digitizer 100 generates a laser pattern that may be projected on or towards a dental item, dentition, or prepared dentition in an oral cavity (in vivo). The intra-oral digitizer 100 may remotely generate the laser pattern and relay the pattern towards the dental item or items in vivo. The laser pattern may be relayed through relay optics such as prisms, lenses, relay rods, fiber optic cable, fiber optic bundles, or the like. The intra-oral digitizer 100 also may detect or capture light reflected from the dental item in vivo. The intra-oral digitizer 100, or a portion thereof, may be inserted in the oral cavity to project the laser pattern and to detect the reflected laser pattern from the dental item or items in the oral cavity. The captured light may be used to generate data representative of the 3D image of the dentition. The data may be used to display the 3D image. The data also may be used to form a model of the object using known techniques such as milling techniques. The model of the object may be a dental restoration such as a crown, bridge, inlay, onlay, implant or the like. The data also may be used for diagnostic purposes.

[0034] The laser digitizer 100 includes a laser light source 101, a first scanner 102 (x scanner), a second scanner 103 (y scanner), a lens assembly 104, a first reflecting prism 113, a first optics relay 105, a second reflecting prism 107, a third reflecting prism 106, a second optics relay 109, imaging optics assembly 110, imaging sensor 111, and an electronic circuit 112. The intra-oral laser digitizer 100 may be coupled to a processor 119.

[0035] The laser light source 101 may include collimating optics (not shown) that generate a laser beam of light 122 from the light source 101. The collimated light beam 122 is characterized by parallel rays of laser light. The laser beam 122 is projected to the first scanner 102.

[0036] The laser light source 101 may include a laser diode or LED that generates a laser light beam having an elliptical-shaped cross-section. The collimating optics may be configured to circularize the elliptical beam and to generate a circular spot. The circular spot may be used to scan a uniform line across the surface of the object 108. The laser diode may be any commercially available laser diode configured to emit a laser light beam, such as the Blue Sky Research Mini-Laser 30 mWatt laser with 0.6 mm collimated beam, model number Mini-635D3D01-0.

[0037] The laser light source 101 also may modulate the laser light beam. The laser light source 101 may be coupled

to a modulator that adjusts or interrupts light flow from the source at high modulation or switching rate. The modulation may be in the range of substantially 1 kHz to substantially 20 MHz. A scan pattern may be generated on the object, by modulating the laser light source **101**.

[0038] The first scanner **102** includes an x-scanner mirror having a substantially flat reflecting surface. The reflecting surface of the x-scanner mirror, may be rectangular-shaped having dimensions approximately 1.5 mm by approximately 0.75 mm. The laser beam **122** from the light source **101** may have a width no greater than the smallest dimension of the first scanner **102**. For example, the width of the laser beam may be approximately 0.6 mm. The beam of light **122** from the laser light source **101** is incident upon the reflecting surface of the first scanner **102**.

[0039] The second scanner **103** includes a y-scanner mirror having a substantially flat reflecting surface. The reflecting surface of the y-scanner mirror, may be rectangular-shaped having dimensions approximately 1.5 mm by approximately 0.75 mm. The reflecting surfaces of the x-scanner and the y-scanner may be mirrors or the like.

[0040] FIG. 2 illustrates the second scanner **103** positioned substantially orthogonal to the first scanner **102**. The first scanner **102** directs the beam of light **122** towards the second scanner **103**. The beam **122** directed from the first scanner **102** is incident upon the reflecting surface of the second scanner **103**. The first scanner **102** directs the beam **122** along an arc onto the reflecting surface of the second scanner **103**. The reflective surface of the first scanner **102** may be rotated through an axis of rotation to create the arc on the reflective surface of the second scanner **103**. Together, the reflecting surfaces of the first scanner **102** and the second scanner **103** form a two-axis scanner assembly **116**. The reflective surface of the second scanner **103** rotates through the y-axis to direct a two-axis scanned beam **124** in an orthogonal direction.

[0041] The scanned beam **124** is incident upon the lens assembly **104**. The lens assembly **104** focuses the scanned beam **124** through the first reflecting prism **113**. The first reflecting prism **113** directs a scanned image **125** to the first optics relay **105**.

[0042] FIG. 3 illustrates the first optics relay **105** relaying the scanned image **125** to the second reflecting prism **107**. The second reflecting prism **107** may be inserted into an oral cavity to project the laser pattern toward one or more dental items to be imaged. The first optics relay **105** transmits the laser pattern generated by the light source **101**, the first and second scanner **102**, **103** and the lens assembly **104** to a remote location, such as an oral cavity. The second reflecting prism **107** projects a scanned beam **114** towards the object **108** so that a light pattern may be projected on the object **108**. The first optics relay **105** may be any commercially available relay optics system. The first optics relay **105** may be a relay lens such as a GRIN lens, a fiber optic cable, a fiber optic bundle, or similar device for relaying an optical image over a distance **L1**. An example of a first optics relay **105** is a GrinTech rod lens with part number 12534082-4C-9 attached to the GrinTech objective grin lens with part number CR1032-2.

[0043] As shown in FIG. 4, a reflection **115** of the scanned beam **114** from the surface of the object **108** is captured

through the third reflecting prism **106** to relay captured reflection **126**. The third reflecting prism **106** may be inserted into an oral cavity to detect or capture reflections of the laser pattern from the one or more dental items to be imaged. The second optics relay **109** transmits captured reflection **126** for a distance **L2** from the oral cavity to the imaging optics assembly **110**. The captured reflection **126** from the object **108** is imaged and focused by the imaging optics **110** to provide a focused beam **127**. The focused beam **127** is projected towards the imaging sensor **111**. The imaging sensor **111** may be a CCD sensor, a CMOS sensor, or other light sensitive device or array of light sensitive devices. The second optics relay **109** may be any commercially available relay optics system. The second optics relay **109** may be a relay lens such as a GRIN lens, a fiber optic cable, a fiber optic bundle, or similar device for relaying an optical image over a distance **L2**. An example of the second optics relay **109** is the GrinTech rod lens with part number 12534082-4C attached to the GrinTech objective grin lens with part number CR1032-2.

[0044] The imaging sensor **111** may be coupled with electrical circuit **112**. The electrical circuit **112** may include electrical and electronic components suitable for processing electrical signals of the intra-oral digitizer **100**. The electrical circuit **112** may be located or enclosed within a suitable enclosure. The enclosure may be a hand-held enclosure or have a form factor suitable for being handheld, for enclosing the electrical circuit **112** and for manipulating the intra-oral digitizer **100** in vivo. The enclosure and electrical circuit may be remotely located from the second and third reflecting prisms **107**, **106**. The electrical circuit **112** may modulate the light source **101**, and drive the scanning mirrors **102** and **103**. The electrical circuit also may gather electronic data received from the imaging sensor **111**. The electrical circuit also may perform additional processing and communication with an external processor **119** via a cable or wireless or some other communications link.

[0045] FIG. 5 illustrates an imaging optics system **120** of the laser digitizer **100**. The imaging optics system **120** may include the third reflecting prism **106**, the second optics relay **109**, the imaging optics **110** and the imaging sensor **111**. The imaging optics system **120** generates a digital signal representative of the captured reflection **126**.

[0046] FIG. 6 illustrates the projection optics system **121**, including the lens assembly **104**, the first reflecting prism **113**, the first optics relay **105**, and the second reflecting prism **107**. The projection optics system **121** may project the scanned image in the direction of the the object **108** so as to project the laser pattern in vivo.

[0047] FIG. 7 illustrates a front view of a portion of the intra-oral laser digitizer **100**. The scanned beam **114** is directed from the projection optics system **121** in the direction of the object **108**. Reflected light **115** is captured or detected by the imaging optics system **120**. The imaging optics system **120** may be characterized by a coordinate system having axes X, Y, Z and the projection optics system **121** may be characterized by a coordinate system having axes X'Y'Z'. The Z' axis projects vertically from a center of the second reflecting prism **107** to the object **108**, and Z is the axis projected vertically from the surface of the object at **108** to a center of the third reflecting prism **108**. The X' axis is orthogonal to the Z' axis and in a horizontal plane with

respect to the front of the intra-oral device **100**. The X axis is orthogonal to the Z axis. The Y' axis may be defined according to the X' axis and the Z' axis in a right-handed coordinate system, as illustrated in the top view of the second reflecting prism **106** and the third reflecting prism **107**, as illustrated in **FIG. 8**. The Y axis may be defined according to the X' axis and the Z' axis in a right-handed coordinate system, as illustrated in the top view of the second reflecting prism **106** and the third reflecting prism **107**, as illustrated in **FIG. 8**.

[0048] An angle between the Z axis and Z' axis may be designated as  $\theta$ . A distance from a center of the third reflecting prism **106** to the point on the object **108** may be referred to as d1 and a distance from the center of the third reflecting prism **106** to a top of a depth of focus region may be referred to as d2.

[0049] **FIG. 9** illustrates a two-axis scanner assembly **116**. The two-axis scanner assembly may include the first scanner **102** and the second scanner **103**. The first scanner **102** includes a reflective surface that rotates about axis **117**. The reflective surface of the first scanner **102** directs the light to the reflecting surface of the second scanner **103**. The reflective surface of the second scanner **103** rotates about the axis **118**.

[0050] The reflective surfaces of the scanners **102** and **103** may be rotatably coupled with a respective motor, other electromagnetic driving mechanism, or electrostatic driving mechanism such as magnets, coils or other electromagnetic coupling that control a rotational movement of the corresponding reflective surface to effect the scanning of the collimated light beam.

[0051] The two-axis scanner **116** redirects, or scans, the collimated light beam to form a scanned light beam **114** having a position that varies over time. The scanned beam **114** is directed by the two-axis scanner **116** to the lens assembly **104** and the first optics relay **105**. The two-axis scanner **116** redirects the collimated light beam in at least two or more axes **117**, **118** where each axis is substantially perpendicular to the axis of the collimated light beam. The first and second scanners **102**, **103** may have essentially perpendicular axes, and may be essentially orthogonal with respect to each other. The scanners **102**, **103** also may be positioned at an arbitrary angle relative to each other.

[0052] Additional scanners also may be included to scan the collimated light beam. The scanners **102**, **103** may be positioned orthogonally so that the collimated laser beam incident on the reflectors may be scanned or redirected in at least two axes. The first scanner **102** scans the beam along one axis, such as an x-axis. The second scanner **103** may be positioned so that the beam along the x-axis incident upon the second scanner **103** may be scanned along an orthogonal direction to the x-axis, such as a y-axis. For example, the first and second scanner **102**, **103** may be positioned orthogonal with respect to each other so that the first scanner **102** scans the beam along the x-axis and the second scanner **103** scans the beam along an orthogonal direction to the x-axis, such as a y-axis.

[0053] The first scanner **102** also may have a spinning polygon mirror such that the rotatable second reflector **103** and the spinning polygon reflector **102** together also are configured to scan the laser beam in two axes. The spinning

polygon mirror **102** may scan the collimated light beam along an x-axis and the rotatable mirror **103** may scan the collimated light beam along a y-axis. Each axis, the x-axis and y-axis, may be substantially orthogonal with one another to generate a scanned light beam along two substantially orthogonal axes.

[0054] The two-axis scanner **116** also may include a single reflecting surface that scans a beam of light along two axes. The reflecting surface may be driven electromagnetically or electro-statically to rotate the reflecting surface about two essentially orthogonal axes individually or simultaneously.

[0055] The two-axis scanner **116** may include one or more Microelectro-mechanical systems ("MEMS"), which have reflecting surfaces that may be driven electromagnetically or electro-statically or using a piezo crystal or otherwise mechanically to rotate the reflecting surface about two essentially orthogonal axes individually or simultaneously.

[0056] The two-axis scanner **116** also may include a programmable position controller. The position controller may be a component of the two-axis scanner **116** or may be incorporated with the electronic circuit **112**. The controller may control movement of the scanners **102**, **103** by providing control signals to the drive mechanisms of the reflective surfaces of the scanners **102**, **103**. The controller controls the movement of the scanners **102**, **103** so that the collimated laser beam is redirected to provide to a scan sequence. The coordinate system for the two-axis scanner **116** is referred to as X'Y'Z'.

[0057] As shown in **FIGS. 7 and 8**, the object **108** to be imaged is positioned within a field of view of projection optics **121** and the imaging optics system **120**. The projection optics **121** is positioned at the angle  $\theta$  with respect to an optical axis of the imaging optics system **120** so that when the focused dot is scanned across the surface of the object **108** the light is reflected towards the imaging optics system **120** at angle  $\theta$ . The two-axis scanner **116** moves the scanned beam **114** so that the focus point of the laser dot from the projection optics **121** traverses through a pattern across the surface of the object **108**.

[0058] The imaging optics system **120** may be configured and/or positioned to have a field of view that includes the focused laser dot projected on the object **108**. The imaging optics system **120** detects the laser dot as it is scanned across the surface of the object **108**. The imaging optics system **120** includes an image sensor **111** that is sensitive to the light reflected from the object **108**. The imaging optics system **120** may include an imaging lens **110** and an image sensor **111** and the second optics relay **109** and a prism or fold mirror **106**. The imaging lens **110** is configured to focus the light reflected from the object **108** towards the image sensor **111**. Based on a light detected from the object **108**, the image sensor **111** generates an electrical signal representative of the surface characteristics (e.g., the contours, shape, arrangement, composition, etc.) of the object **108**.

[0059] The image sensor **111** captures an image of the scanned surface of the object **108**. The image sensor **111** may be a photo-sensitive or light sensitive device or electronic circuit capable of generating signal representative of intensity of a light detected. The image sensor **111** may include an array of photodetectors. The array of photodetectors may be a charge coupled device ("CCD") or a CMOS imaging

device, or other array of light sensitive sensors capable of generating an electronic signal representative of a detected intensity of the light. The image sensor **111** may comprise a commercially available CCD or CMOS high resolution video camera having imaging optics, with exposure, gain and shutter control, such as the Silicon Imaging USB Camera SI-1280F-U.

[0060] Each photo-detector of the image sensor **111** generates an electric signal based on an intensity of the light incident or detected by the photo-detector. In particular, when light is incident to the photo-detector, the photo-detector generates an electrical signal corresponding to the intensity of the light. The array of photo-detectors includes multiple photo-detectors arranged so that each photo-detector represents a picture element, or pixel of a captured image. Each pixel may have a discrete position within the array. The image capture instrument **120** may have a local coordinate system, XY such that each pixel of the scanned pattern corresponds to a unique coordinate (x,y). The array may be arranged according to columns and rows of pixels or any other known arrangement. By virtue of position of the pixel in the array, a position in the image plane may be determined. The imaging optics system **120** converts the intensity sensed by each pixel in the image plane into electric signals that represent the image intensity and distribution in an image plane.

[0061] The CMOS image sensor may be configured to have an array of light sensitive pixels. Each pixel minimizes any blooming effect such that a signal received by a pixel does not bleed into adjacent pixels when the intensity of the light is too high.

[0062] The two-axis scanner **116** may be configured to scan the laser beam **114** across the surface of the object **108** via the projection optics **121** in various patterns. The pattern may cover a portion of the surface of the object **108** during a single exposure period. The pattern also may include one or more curves or any known pattern from which the characteristics, elevations and configurations of the surface of the object **108** may be obtained.

[0063] During an exposure period, an image of a portion of the surface of the object is captured. The beam **114** scans the object **108** via the two-axis scanner **116** and the projection optics **121** in a selected pattern, allowing the imaging sensor **111** to detect the light reflected from object **108**. The image sensor **111** generates data representative of the surface characteristics, contours, elevations and configurations of the scanned portion or captured image. The data representation may be stored in an internal or external device such as a memory.

[0064] FIG. 10 illustrates an example of a scanned pattern of light **1048** as viewed from a substantially flat surface. The scanned pattern **1048** may include multiple curves **1050-1055** that are generated by the scanner **116**. A portion of the curves **1050-1051** may be essentially parallel to each other. The curves **1050-1055** also may represent or include a connected series of points or curvilinear segments where a tangent vector n at any single point or segment obeys the following rule:

$$|n \cdot R| = 0 \quad (1)$$

[0065] where R is a triangulation axis that is substantially parallel to Y and Y' and passes through an intersection of an

axial ray from the third reflecting prism **106** of the image optics system **120** and an axial ray from the second reflecting prism **107** of the optical projection system **121**. Accordingly, the angle between the tangent n at any point or segment of the curve and the triangulation axis R is not 90 degrees. Each curve **1050-1055** also may have a cross-sectional intensity characterized by a function that may have a sinusoidal variation, a Gaussian profile, or any other known function for cross-sectional intensity. In an embodiment, a minimum angle between a valid ray between the second reflecting prism **107** relative to a valid axial ray of the third reflecting prism **106** is non-zero.

[0066] During a subsequent scan period, the beam **114** is scanned in a pattern across an adjacent portion of the object **108** and an image of the adjacent portion is captured. The scanned beam **114** may scan a different area of the surface of the object **108** during subsequent exposure periods. After several exposure periods in which the beam **114** is scanned across the various portions of the object **108** and images of those scanned portions captured, a substantial portion of the object may be captured.

[0067] The processor **119** may be coupled to the imaging optics system **120** and configured to receive the signals generated by the image capture instrument **120** that represent images of the scanned pattern on the object **108**. The processor **119** may process and display the signals generated by the image optics system **120**. The processor **119** also may be coupled to the laser light source and control selected or programmed applications of the laser light. The processor **119** also may be coupled with the two-axis scanner **116** and programmed to control the scanning of the collimated light.

[0068] The image optics system **120** may be characterized by a local coordinate system X, Y, Z, where the X and Y coordinates may be defined by the image imaging optics system **120**. A value for the Z coordinate may be based on the distance  $d_1$  and  $d_2$  so that  $d_1 \leq z \leq d_2$ . A point from a projected curve incident to a plane perpendicular to Z will appear to be displaced in the X direction by  $\Delta x$ .

[0069] Based on a triangulation angle, the following condition may exist:

$$\Delta z = \frac{\Delta x}{\tan \theta} \quad (2)$$

[0070] For a given curve (e.g. curve **1050**) in the projection pattern there may be unique relations  $\theta(y)$ ,  $z_{\text{base}}(y)$  and  $x_{\text{base}}(y)$ . The relations  $\theta(y)$ ,  $z_{\text{base}}(y)$  and  $x_{\text{base}}(y)$  relations may be determined through calibration. The calibration may be performed for example by observing the curve **1050** as projected on a plane surface. The plane surface may be perpendicular to the imaging optics system **120** at two or more distances d along the Z axis from the image optics system **120**. For each y value along the curve **1050**, using at least two such curves with known z values of  $z_1$  and  $z_2$ , where  $z_1 < z_2$ ,  $\Delta z$  may be computed as  $\Delta z = z_2 - z_1$ . A value  $\Delta x$  may be observed using imaging optics system **120**. Using equation (2),  $\theta(y)$  may be computed. The corresponding value  $z_{\text{base}}(Y)$  may be set equal to  $z_1$ . The corresponding value  $x_{\text{base}}(Y)$  may be equal to an x value at the point y on

the curve corresponding to  $z_1$ . Additional curves may be used to improve accuracy of through averaging or interpolation.

[0071] FIG. 11 illustrates the scanned pattern of light 1148 projected on the object 1180 to be imaged. FIG. 12 illustrates the light pattern reflected from the object 1180 as incident to the image sensor 1234. For the observed projected curves 1250-1255 on the object, each curve corresponds to one of the curves 1150-1155 shown in FIG. 11 and a corresponding one of the curves 1050-1055 shown FIG. 10. Accordingly, for each curve 1250-1255, the corresponding relations  $\theta(y)$ ,  $z_{\text{base}}(Y)$  and  $x_{\text{base}}(y)$  may be selected that were pre-computed during a calibration. For each point  $(x_{\text{observed}}, y_{\text{observed}})$  on each curve 1250-1255,

$$\Delta x = x_{\text{observed}} - x_{\text{base}}(y_{\text{observed}}) \quad (3)$$

[0072] Equation (2) may be used to determine  $\Delta z$  using  $\theta(Y_{\text{observed}})$ , and consequently

$$z_{\text{observed}} = \Delta z + z_{\text{base}}(y_{\text{observed}}) \quad (4)$$

[0073] The collection of points  $(x_{\text{observed}}, y_{\text{observed}}, z_{\text{observed}})$  obtained, form a 3D image of the object 1180.

[0074] A maximum displacement for a curve may be determined by:

$$\Delta x = (d_1 - d_2) \tan \theta \quad (4)$$

[0075] A maximum number  $n_{\text{max}}$  of simultaneously distinguishable curves 1050 may be determined according to  $n_{\text{max}} = X_{\text{max}} / \Delta x$  or equivalently

$$n_{\text{max}} = \frac{X_{\text{max}}}{(d_1 - d_2) \tan \theta_{\text{max}}} \quad (5)$$

[0076] The number  $n_{\text{max}}$  increases with a decreasing depth of field  $d_1 - d_2$  and increases with a smaller  $\theta_{\text{max}}$ . The accuracy of the determination also may decrease with smaller  $\theta_{\text{max}}$  values.

[0077] Where the number of curves  $n$  exceeds  $n_{\text{max}}$ , any ambiguity in the labeling of the lines may be resolved by associating the observed curves into groups of adjacent curves. For each group of adjacent curves, if at least one curve is correctly labeled, then all other curves in that group may be labeled using adjacency. A method to determine the correct labeling of at least one curve in a group may include considering a second pattern where the number of curves is less than  $n_{\text{max}}$  and may be at an angle relative to the first pattern. The curves of the second pattern may be properly labeled, and intersections of the curves of the second pattern with the curves of the first pattern may be used to deduce labeling of some subset of the curves in the first pattern. This may be repeated with additional patterns until all curves are correctly labeled.

[0078] FIG. 13 illustrates scanned lines 1350-1352 on the surface of an object. The scanned line 1350 has associated with it a region bounded by the boundary curves 1360 and 1362. The region bounded by boundary lines 1360 and 1362 is determined by a pre-scan event or calibration data, so that the scanned line 1350 may be identified separately from other scanned lines, such as an adjacent line 1352. Adjacent line 1352 is associated with it its own region bounded by 1364 and 1366. Multiple scanned lines may be projected

simultaneously, where each scanned line is uniquely identified, even when projected onto a surface that is not substantially flat.

[0079] FIG. 14 illustrates an example of a pattern-projection system 1470. The pattern-projection system 147 may be incorporated with, part of or a component of the electrical circuit 112. The pattern-projection system 1470 includes a scanner mirror driver circuit 1472 and a laser driver circuit 1474. The mirror driver circuit 1472 includes a RAM-based arbitrary waveform generator (AWG) 1476, 1477 and a transconductance power amplifier stage 1478, 1480 corresponding to a scanner 1482, 1483.

[0080] The AWG 1476 corresponding to a high speed scanner 1482 includes a 16-entry waveform table 1484 and a 12-bit digital-to-analog converter (DAC) 1486. The waveform table 1484 may be incremented at approximately 320 KHz to produce a sinusoidal waveform of approximately 20 KHz.

[0081] The AWG 1477 corresponding to a low-speed scanner 1483 includes a 666-entry waveform table 1485 and a 12-bit DAC 1487. The waveform table 1485 is incremented once per high-speed mirror cycle to produce a sinusoidal waveform of approximately 30 Hz. The two AWGs 1476, 1477 create a repeating raster pattern at approximately 30 frames per second. Electrical signals synchronize a camera system to the scanner driver. A reference input to each DAC 1486, 1487 is driven by a variable voltage 1492, 1493 to dynamically adjust the horizontal and vertical dimensions of the raster.

[0082] The high-speed scanner 1482 is driven at a resonance frequency in the range of about 20 KHz. A position feedback signal of the scanner 1482 may be used with a closed-loop control using a DSP 1495 and a DDS 1496 to adjust drive frequency of the drive signal to track variation in the resonance frequency. The frame rate of the raster pattern may change with the high-speed resonance frequency of the scanner 1482. An example of the DSP includes model number TMS320LF2407A by Texas Instruments. An example of the DDS includes model number AD9834 by Analog Devices.

[0083] The laser driver circuit 1470 may include a multiple-bank random access memory (RAM)-based pattern table 1488 and a laser diode current modulator 1490. The RAM-based pattern table 1488 includes multiple banks of memory, where each bank includes a bit-mapped pixel image to be displayed during a single-pattern frame. A counter synchronized with the raster of the scanner raster generator accesses the pattern table 1488 and to present the pixel data to the laser diode current modulator 1490 to produce a repeating pattern. Each bank of the pattern table 1488 may be loaded with a discrete pattern. Multiple single-pattern frames may be combined into repeating multiple-frame sequences with linked-list mechanism.

[0084] FIG. 15 illustrates a laser digitizer 1500 configured as an optical coherence tomography ("OCT") or confocal sensor. The laser digitizer includes a fiber-coupled laser 1511. The laser source 1511 may be a low coherence light source coupled to a fiber optic cable 1510, coupler 1509 and detector 1501. The coupler, an optical delay line 1505 and reflector 1504 return delayed light to the coupler 1509. The coupler 1509 splits the light from the light source into two

paths. The first path leads to the imaging optics **1506**, which focuses the beam onto a scanner **1507**, which steers the light to the surface of the object. The second path of light from the light source **1511** via the coupler **1509** is coupled to the optical delay line **1505** and to the reflector **1504**. This second path of light is of a controlled and known path length, as configured by the parameters of the optical delay line **1505**. This second path of light is the reference path. Light is reflected from the surface of the object and returned via the scanner **1507** and combined by the coupler **1509** with the reference path light from the optical delay line **1505**. This combined light is coupled to an imaging system **1501** and imaging optics **1502** via a fiber optic cable **1503**. By utilizing a low coherence light source and varying the reference path by a known variation, the laser digitizer provides an Optical Coherence Tomography (OCT) sensor or a Low Coherence Reflectometry sensor. The focusing optics **1506** may be placed on a positioning device **1508** in order to alter the focusing position of the laser beam and to operate as a confocal sensor.

**[0085]** Although embodiments of the invention are described in detail, it should be understood that various changes, substitutions and alterations can be made hereto without departing from the spirit and scope of the invention as described by the appended claims. The laser source may include a laser or LED, and the collimating optics may include optics that circularize the generally elliptical beam produced by such sources. This system may produce a circular spot on the object to provide a generally uniform line when the beam scanned across the object.

**[0086]** The light source may positioned proximate to the intra-oral laser digitizer remotely through a light guide such as optical fiber. The light source may be remote from the sensor structure and to provide for an intra-oral device having smaller dimensions.

**[0087]** A second light source (LED, incandescent bulb, laser, or other) may provide a background light so that the intra-oral laser digitizer may be used as a standard 2D dental camera. This second light source may be located at or near the imaging optical path. The second light source also may be placed remote to the sensor structure with the light brought to the optical path through a light guide.

**[0088]** The intra-oral system also may include a one- or two-axis tilt sensor. The computer may monitor the angles of the tilt sensor, and the received images of the scanned lines to determine a profile for the object. A one-, two- or three-axis accelerometer may determine approximate position changes of the intra-oral digitizer in one, two or three axes.

**[0089]** The system also may include a laser light source having a high speed modulation system. The modulation system switches the laser on and off at a high rate (typically several MHz), reducing the coherence of the laser source and degree of speckle produced by the laser source on the object.

**[0090]** The scanning system may include a single mirror that scans in two orthogonal axes or other non-parallel arrangement. An example of such a micro-mirror scanner is the bi-axial MEMS scanner of Microvision of Washington. The scanning system may include two mirrors that scan in two orthogonal directions or other non-parallel arrangement.

**[0091]** The imaging sensor may be CMOS sensor or a CCD sensor that captures images at high speeds. A processor processes captured images, such that if the probe moves relative to the object, the software adjusts the captured data so that an accurate digitization occurs. The imaging system may include a small image sensor and objective lens mounted directly at the end of the sensor probe to provide a smaller intra-oral probe through elimination of the relay lenses.

**[0092]** The laser source may include a laser source and line generating optics. This laser source produces one or more lines directed to a one axis laser scanner to provide for a low speed scanner or no scanner based on the line generating optics producing sufficient number of separate line segments.

**[0093]** The imaging system may include an objective, relay lens, asymmetric lens system, and a linear sensor array. A linear sensor array or analog position sensor may be read for each pixel position. The asymmetric lens images the scanning field onto the line detector. The triangulation angle causes the laser spot to be imaged onto different elements of the line detector as the object height changes, allowing fast scanning of the object.

**[0094]** A series of imaged laser segments on the object from a single sample position interlace between two or multiple 3D maps of the sample from essentially the same sample position. The time period to measure each interlaced 3D map is reduced to a short interval and relative motion effects between the intra-oral device and the patient are reduced. The interlaced 3D maps may be aligned with software to produce an effective single view dense 3D point cloud that has no motion induced inaccuracies or artifacts. For example, in a 10 step interlacing scheme, each image may be captured in  $\frac{1}{30}$ <sup>th</sup> of a second. When scanning over 0.3 seconds, the present invention reduces affects of operator motion. The motion of the operator between each subframe may be tracked mathematically through reference points in the dataset itself. The operator motion is removed in subsequent analysis, allowing a system with a framerate significantly lower than would otherwise be required.

**[0095]** Multiple dense 3D point clouds also may be acquired from approximately the same position, and mathematically aligned (i.e., moved relative to each other to minimize the distance between them so as to cause related features in each to become superimposed), and statistical methods used to further improve the accuracy of the data (for example, Gaussian filtering).

**[0096]** A low resolution pre-scan of the surface determines approximate geometry. Referring to this pre-scan, an approximate envelope of subsequent laser lines is determined by performing inverse calculation of a laser line centroid to 3D coordinate. Since these envelopes are not rectangular and combined with the assumption that the surface does not change dramatically locally one can greatly increase the number of simultaneous lines projected on the surface and identifiable in the image, increasing the effective scanning rate. In an example of N lines being scanned simultaneously with a system capable of processing F frames per second, an effective F\*N frames per second processing rate, or multiplied by a factor of N, may be achieved.

**[0097]** The imaging system may be located remotely from the imaging sensor. Through relay optics such as a coherent

fiber imaging bundle, the scanning system may be located remotely from the imaging sensor. The Fourier transform of the object image is transferred through the fiber imaging bundle. By transferring the Fourier transform through the fiber bundle, more of the high frequency components of the object image remain. Also, the effects of the fiber bundle can be removed by removing the frequency components from the Fourier transformed image, which corresponds to the fiber bundle.

**[0098]** While various embodiments of the invention have been described, it will be apparent to those of ordinary skill in the art that many more embodiments and implementations are possible within the scope of the invention. Accordingly, the invention is not to be restricted except in light of the attached claims and their equivalents.

What is claimed is:

1. An intra-oral laser digitizer comprising:
  - a light source having collimating optics configured to generate a collimated beam of light;
  - a scanner optically coupled to the light source and configured to scan the collimated beam along at least two axes;
  - an optics relay coupled to the scanner and configured to relay the scanned, collimated beam towards a remote object to be imaged;
  - an image optics system having an optical axis configured to detect a reflection of the scanned beam from the object at an angle  $\theta$  with respect to the optics relay and to generate data representative of a surface of the object based on the reflected beam; and
  - a processor coupled to the scanner and the image optics system configured to generate a three-dimensional image of the object based on the data.
2. The intra-oral laser digitizer of claim 1 where the light source comprises a laser LED.
3. The intra-oral laser digitizer of claim 1 where the scanner comprises a plurality of mirrors.
4. The intra-oral laser digitizer of claim 3 where the image optics system comprises:
  - an image sensor configured to detect a triangulation image of the object, the triangulation image based on a plurality of curves generated by scanning the beam of light on the object during an exposure period; and
  - an imaging lens system configured to focus the plurality of curves on the image sensor.
5. The intra-oral laser digitizer of claim 4 where the processor is configured to merge multiple images of the object to generate a three-dimensional map of the object.
6. The intra-oral laser digitizer of claim 5 where the object comprises any one of an in vivo dental item, a dental preparation, a dental model, a dental mold, or a dental casting.
7. The intra-oral laser digitizer of claim 1 where the scanner comprises a single mirror configured to scan the light along at least two-axes.
8. The intra-oral laser digitizer of claim 1 where the scanner comprises a rotatable mirror and a spinning polygon mirror.

9. The intra-oral laser digitizer of claim 1 where the scanner further comprises a programmable position controller configured to control the scan of the collimated laser beam in a programmed scan sequence.

10. The intra-oral laser digitizer of claim 1 where the known pattern comprises a plurality of curves each is substantially parallel to each other.

11. The intra-oral laser digitizer of claim 1 where the laser light source comprises a low coherence light source, the reflected light from the object being compared with light from the low coherence source reflected from a known variable path length.

12. The intra-oral laser digitizer of claim 1 further comprising a voice-recognition means for controlling operation of the intra-oral laser digitizer in response to voice commands of an operator.

13. A dental imaging system, comprising:

means for generating a collimated laser beam of light;

scanner means for generating a multi-axis collimated light beam;

beam relaying means for relaying the collimated light beam towards an object to be imaged, the object to be imaged being remotely located from the means for generating a collimated laser beam of light;

image capturing means for detecting reflections of the a focused beam projected on an object; and

processor means coupled to the scanner means and the image capturing means for generating a three-dimensional image of the object.

14. The laser digitizer of claim 13 where the scanning means scans the beam across the object in a selected pattern via beam relaying means.

15. The laser digitizer of claim 13 where the image capturing means comprises:

an image sensor configured to detect a triangulation image of the object, where the triangulation image is based on a pattern of scanned lasers dots across the surface of the object during an exposure period; and

an imaging capturing relay means to capture a reflection of the pattern from the object and relay the captured reflection to the image sensor.

16. The laser digitizer of claim 15 where the beam relaying means comprises an optical relay rod lens.

17. A method for generating a three-dimensional visual image of an in vivo object comprising:

generating a multi-axis collimated beam of light, the collimated beam of light being generated remotely from the object;

scanning the multi-axis collimated beam of light, from a first position with respect to the object, in a second pattern, where the pattern includes a plurality of substantially parallel curves having curvilinear segments;

capturing an image of a reflection of the pattern from the object during an exposure period; and

determining a map of the surface of the object based on the captured image.



**18.** The method of claim 17 where the act of scanning further comprises relaying the multi-axis collimated beam of light to an object in oral cavity.

**19.** The method of claim 17 further comprising the acts of:

scanning the multi-axis collimated beam of light, from a second position with respect to the object, in a predetermined pattern, where the pattern includes a plurality of substantially parallel curves having a curvilinear segments;

capturing an image of a reflection of the pattern from the object in the second position; and

merging the captured image from the first position with the captured image from the second position.

**20.** The method of claim 17 where the second pattern is substantially similar to the first pattern.

\* \* \* \* \*