



US011697011B2

(12) **United States Patent**
Merritt et al.

(10) **Patent No.:** **US 11,697,011 B2**

(45) **Date of Patent:** **Jul. 11, 2023**

(54) **HEMOSTASIS VALVES AND METHODS OF USE**

(71) Applicant: **Inari Medical, Inc.**, Irvine, CA (US)

(72) Inventors: **Benjamin E. Merritt**, San Clemente, CA (US); **John C. Thress**, Capistrano Beach, CA (US); **Paul Lubock**, Monarch Beach, CA (US)

(73) Assignee: **Inari Medical, Inc.**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **17/705,189**

(22) Filed: **Mar. 25, 2022**

(65) **Prior Publication Data**

US 2022/0211992 A1 Jul. 7, 2022

Related U.S. Application Data

(63) Continuation of application No. 17/226,318, filed on Apr. 9, 2021, which is a continuation of application (Continued)

(51) **Int. Cl.**

A61M 39/06 (2006.01)

A61B 17/3207 (2006.01)

(52) **U.S. Cl.**

CPC **A61M 39/0613** (2013.01); **A61B 17/3207** (2013.01); **A61M 2039/062** (2013.01); **A61M 2039/0673** (2013.01)

(58) **Field of Classification Search**

CPC **A61M 2039/062**; **A61M 2039/0673**; **A61M 39/0613**; **F16K 7/02**; **F16K 7/08**; **F16K 7/04**

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,846,179 A 8/1958 Monckton

2,955,592 A 10/1960 Maclean

(Continued)

FOREIGN PATENT DOCUMENTS

AU 2015210338 8/2015

CN 102186427 9/2011

(Continued)

OTHER PUBLICATIONS

European Patent Application No. 13838945.7, Extended European Search Report, 9 pages, dated Apr. 15, 2016.

(Continued)


Primary Examiner — Quynh-Nhu H. Vu

(74) *Attorney, Agent, or Firm* — Perkins Coie LLP

(57) **ABSTRACT**

Devices, systems, and methods for sealing medical devices, particularly during intravascular access, are disclosed herein. Some aspects relate to a hemostatic valve for sealing a wide range of medical devices, such as catheters, wires, embolectomy systems. The valve can include an elongate member having a first end, a second end, and a central lumen extending therebetween. A reinforcement structure extends along at least a portion of the elongate member and is coupled to the elongate member. A shell defining a first aperture and a second aperture may be included, which first and second apertures can be fluidly coupled by the elongate member. A tensioning mechanism is coupled to the shell and to the elongate member, the tensioning mechanism can be moveable between a first configuration wherein the tensioning mechanism is collapsed and the central lumen is sealed and a second configuration wherein the central lumen is open.

9 Claims, 10 Drawing Sheets

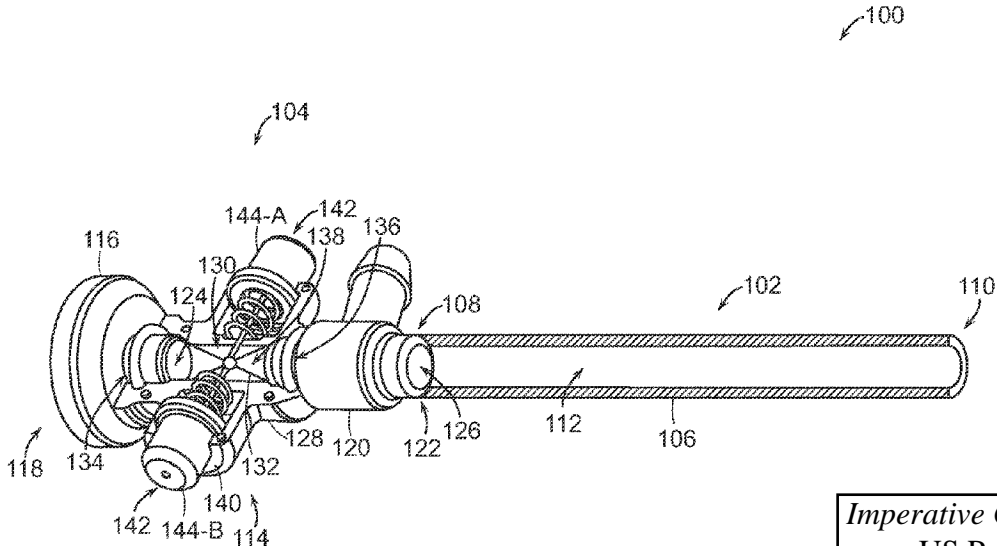

Imperative Care v. Inari Medical
US Patent 12,109,384
Imperative Care Ex. 1022

Related U.S. Application Data

No. 16/117,519, filed on Aug. 30, 2018, now Pat. No. 11,000,682.

(60) Provisional application No. 62/554,931, filed on Sep. 6, 2017.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,088,363 A 5/1963 Sparks
 3,197,173 A 7/1965 Taubenheim
 3,435,826 A 4/1969 Fogarty
 3,515,137 A 6/1970 Santomieri
 3,675,657 A * 7/1972 Gauthier A61B 17/132
 606/203
 3,892,161 A 7/1975 Sokol
 3,923,065 A 12/1975 Nozick et al.
 4,030,503 A 6/1977 Clark, III
 4,034,642 A 7/1977 Iannucci et al.
 4,222,380 A 9/1980 Terayama
 4,243,040 A 1/1981 Beecher
 4,287,808 A 9/1981 Leonard et al.
 4,324,262 A 4/1982 Hall
 4,393,872 A 7/1983 Reznik et al.
 4,469,100 A 9/1984 Hardwick
 4,523,738 A 6/1985 Raftis et al.
 4,551,862 A * 11/1985 Haber A61F 2/0036
 600/491
 4,604,094 A 8/1986 Shook
 4,611,594 A 9/1986 Grayhack et al.
 4,643,184 A 2/1987 Mobin-Uddin
 4,646,736 A 3/1987 Auth et al.
 4,650,466 A 3/1987 Luther
 4,776,337 A 10/1988 Palmaz
 4,790,812 A 12/1988 Hawkins, Jr. et al.
 4,863,440 A 9/1989 Chin et al.
 4,870,953 A 10/1989 DonMichael et al.
 4,883,458 A 11/1989 Shiber
 4,886,062 A 12/1989 Wiktor
 4,890,611 A 1/1990 Monfort et al.
 4,898,575 A 2/1990 Fischell et al.
 4,946,440 A 8/1990 Hall
 4,960,259 A 10/1990 Sunnavader
 4,978,341 A 12/1990 Niederhauser
 5,059,178 A 10/1991 Ya
 5,100,423 A 3/1992 Fearnot
 5,127,626 A 7/1992 Hilal et al.
 5,129,910 A 7/1992 Phan et al.
 5,135,484 A 8/1992 Wright
 5,154,724 A 10/1992 Andrews
 5,158,533 A 10/1992 Strauss et al.
 5,158,564 A 10/1992 Schnepf-Pesch et al.
 5,192,274 A 3/1993 Bierman
 5,192,286 A 3/1993 Phan et al.
 5,192,290 A 3/1993 Hilal
 5,197,485 A 3/1993 Grooters
 5,329,923 A 7/1994 Lundquist
 5,360,417 A 11/1994 Gravener et al.
 5,364,345 A 11/1994 Lowery et al.
 5,376,101 A 12/1994 Green et al.
 5,383,887 A 1/1995 Nadal
 5,389,100 A 2/1995 Bacich et al.
 5,419,774 A 5/1995 Willard et al.
 5,421,824 A 6/1995 Clement et al.
 5,443,443 A 8/1995 Shiber
 5,456,667 A 10/1995 Ham et al.
 5,476,450 A 12/1995 Ruggio
 5,490,859 A 2/1996 Mische et al.
 5,496,365 A 3/1996 Sgro
 5,527,326 A 6/1996 Hermann et al.
 5,549,626 A 8/1996 Miller et al.
 5,591,137 A 1/1997 Stevens
 5,653,684 A 8/1997 Laptewicz et al.
 5,662,703 A 9/1997 Yurek et al.
 5,746,758 A 5/1998 Nordgren et al.

5,749,858 A 5/1998 Cramer
 5,769,816 A 6/1998 Barbut et al.
 5,782,817 A 7/1998 Franzel et al.
 5,800,457 A 9/1998 Gelbfish
 5,827,229 A 10/1998 Auth et al.
 5,846,251 A 12/1998 Hart
 5,860,938 A 1/1999 Lafontaine et al.
 5,873,866 A 2/1999 Kondo et al.
 5,873,882 A 2/1999 Straub et al.
 5,876,414 A 3/1999 Straub
 5,895,406 A 4/1999 Gray et al.
 5,908,435 A 6/1999 Samuels
 5,911,710 A 6/1999 Barry et al.
 5,911,733 A 6/1999 Parodi
 5,911,754 A 6/1999 Kanesaka et al.
 5,941,869 A 8/1999 Patterson et al.
 5,947,985 A 9/1999 Imram
 5,954,737 A 9/1999 Lee
 5,971,938 A 10/1999 Hart et al.
 5,972,019 A 10/1999 Engelson et al.
 5,974,938 A 11/1999 Lloyd
 5,989,233 A 11/1999 Yoon
 5,993,483 A 11/1999 Gianotti
 6,030,397 A 2/2000 Moneti et al.
 6,066,158 A 5/2000 Engelson et al.
 6,068,645 A 5/2000 Tu
 6,126,635 A 10/2000 Simpson et al.
 6,142,987 A 11/2000 Tsugita
 6,146,396 A 11/2000 Konya et al.
 6,146,403 A 11/2000 St. Germain
 6,152,946 A 11/2000 Broome et al.
 6,156,055 A 12/2000 Ravenscroft
 6,159,230 A 12/2000 Samuels
 6,165,196 A 12/2000 Stack et al.
 6,168,579 B1 1/2001 Tsugita
 6,179,859 B1 1/2001 Bates et al.
 6,221,006 B1 4/2001 Dubrul et al.
 6,228,060 B1 5/2001 Howell
 6,238,412 B1 5/2001 Dubrul et al.
 6,245,078 B1 6/2001 Ouchi
 6,245,089 B1 6/2001 Daniel et al.
 6,254,571 B1 7/2001 Hart
 6,258,115 B1 7/2001 Dubrul
 6,264,663 B1 7/2001 Cano
 6,306,163 B1 10/2001 Fitz
 6,322,572 B1 11/2001 Lee
 6,350,271 B1 2/2002 Kurz et al.
 6,361,545 B1 3/2002 Macoviak et al.
 6,364,895 B1 4/2002 Greenhalgh
 6,368,339 B1 4/2002 Amplatz
 6,383,205 B1 5/2002 Samson et al.
 6,402,771 B1 6/2002 Palmer et al.
 6,413,235 B1 7/2002 Parodi
 6,423,032 B2 7/2002 Parodi
 6,432,122 B1 8/2002 Gilson et al.
 6,451,036 B1 9/2002 Heitzmann et al.
 6,458,103 B1 10/2002 Albert et al.
 6,475,236 B1 11/2002 Roubin et al.
 6,485,502 B2 11/2002 Don Michael
 6,508,782 B1 1/2003 Evans et al.
 6,511,492 B1 1/2003 Rosenbluth et al.
 6,514,273 B1 2/2003 Voss et al.
 6,530,923 B1 3/2003 Dubrul et al.
 6,530,935 B2 3/2003 Wensel et al.
 6,544,276 B1 4/2003 Azizi
 6,544,278 B1 4/2003 Vrba et al.
 6,544,279 B1 4/2003 Hopkins et al.
 6,551,342 B1 4/2003 Shen et al.
 6,564,828 B1 5/2003 Ishida
 6,569,181 B1 5/2003 Burns
 6,575,995 B1 6/2003 Huter et al.
 6,589,263 B1 7/2003 Hopkins et al.
 6,596,011 B2 7/2003 Johnson et al.
 6,602,271 B2 8/2003 Adams et al.
 6,605,074 B2 8/2003 Zadno-azizi et al.
 6,605,102 B1 8/2003 Mazzocchi et al.
 6,610,077 B1 8/2003 Hancock et al.
 6,620,148 B1 9/2003 Tsugita
 6,620,179 B2 9/2003 Brook et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,620,182	B1	9/2003	Khosravi et al.	8,100,935	B2	1/2012	Rosenbluth et al.
6,623,460	B1	9/2003	Heck	8,109,962	B2	2/2012	Pal
6,635,068	B1	10/2003	Dubrul et al.	8,118,829	B2	2/2012	Carrison et al.
6,645,222	B1	11/2003	Parodi et al.	8,197,493	B2	6/2012	Ferrera et al.
6,660,013	B2	12/2003	Rabiner et al.	8,246,641	B2	8/2012	Osborne et al.
6,660,014	B2	12/2003	Demarais et al.	8,261,648	B1	9/2012	Marchand et al.
6,663,650	B2	12/2003	Sepetka et al.	8,267,897	B2	9/2012	Wells
6,692,504	B2	2/2004	Kurz et al.	8,298,257	B2	10/2012	Sepetka et al.
6,699,260	B2	3/2004	Dubrul et al.	8,317,748	B2	11/2012	Fiorella et al.
6,702,830	B1	3/2004	Demarais et al.	8,337,450	B2	12/2012	Fotjik
6,719,717	B1	4/2004	Johnson et al.	RE43,902	E	1/2013	Hopkins et al.
6,755,847	B2	6/2004	Eskuri	8,357,178	B2	1/2013	Grandfield et al.
6,767,353	B1	7/2004	Shiber	8,361,104	B2	1/2013	Jones et al.
6,790,204	B2	9/2004	Zadno-azizi et al.	8,409,215	B2	4/2013	Sepetka et al.
6,800,080	B1	10/2004	Bates	8,486,105	B2	7/2013	Demond et al.
6,818,006	B2	11/2004	Douk et al.	8,491,539	B2	7/2013	Fotjik
6,824,545	B2	11/2004	Sepetka et al.	8,512,352	B2	8/2013	Martin
6,824,550	B1	11/2004	Noriega et al.	8,535,283	B2	9/2013	Heaton et al.
6,824,553	B1	11/2004	Gene et al.	8,535,334	B2	9/2013	Martin
6,830,561	B2	12/2004	Jansen et al.	8,545,526	B2	10/2013	Martin et al.
6,846,029	B1	1/2005	Ragner et al.	8,568,432	B2	10/2013	Straub
6,902,540	B2	6/2005	Porros et al.	8,574,262	B2	11/2013	Ferrera et al.
6,939,361	B1	9/2005	Kleshinski	8,579,915	B2	11/2013	French et al.
6,942,682	B2	9/2005	Vrba et al.	8,585,713	B2	11/2013	Ferrera et al.
6,945,977	B2	9/2005	Demarais et al.	8,608,754	B2	12/2013	Wensel et al.
6,960,189	B2	11/2005	Bates et al.	8,657,867	B2	2/2014	Dorn et al.
6,960,222	B2	11/2005	Vo et al.	8,696,622	B2	4/2014	Fiorella et al.
7,004,931	B2	2/2006	Hogendijk	8,715,314	B1	5/2014	Janardhan et al.
7,004,954	B1	2/2006	Voss et al.	8,721,714	B2	5/2014	Kelley
7,036,707	B2	5/2006	Aota et al.	8,753,322	B2	6/2014	Hu et al.
7,041,084	B2	5/2006	Fotjik	8,771,289	B2	7/2014	Mohiuddin et al.
7,052,500	B2	5/2006	Bashiri et al.	8,777,893	B2	7/2014	Malewicz
7,056,328	B2	6/2006	Arnott	8,784,441	B2	7/2014	Rosenbluth et al.
7,063,707	B2	6/2006	Bose et al.	8,784,442	B2	7/2014	Jones et al.
7,069,835	B2	7/2006	Nishri et al.	8,795,305	B2	8/2014	Martin et al.
7,094,249	B1	8/2006	Thomas et al.	8,795,345	B2	8/2014	Grandfield et al.
7,179,273	B1	2/2007	Palmer et al.	8,801,748	B2	8/2014	Martin
7,223,253	B2	5/2007	Hogendijk	8,808,259	B2	8/2014	Walton et al.
7,232,432	B2	6/2007	Fulton, III et al.	8,814,927	B2	8/2014	Shin et al.
7,244,243	B2	7/2007	Lary	8,820,207	B2	9/2014	Marchand et al.
7,285,126	B2	10/2007	Sepetka et al.	8,826,791	B2	9/2014	Thompson et al.
7,300,458	B2	11/2007	Henkes et al.	8,828,044	B2	9/2014	Aggerholm et al.
7,306,618	B2	12/2007	Demond et al.	8,833,224	B2	9/2014	Thompson et al.
7,320,698	B2	1/2008	Eskuri	8,845,621	B2	9/2014	Fotjik
7,323,002	B2	1/2008	Johnson et al.	8,852,226	B2	10/2014	Gilson et al.
7,331,980	B2	2/2008	Dubrul et al.	8,939,991	B2	1/2015	Krolik et al.
7,534,234	B2	5/2009	Fotjik	8,945,143	B2	2/2015	Ferrera et al.
7,578,830	B2	8/2009	Kusleika et al.	8,945,172	B2	2/2015	Ferrera et al.
7,621,870	B2	11/2009	Berrada et al.	8,956,384	B2	2/2015	Berrada et al.
7,674,247	B2	3/2010	Fotjik	8,992,504	B2	3/2015	Castella et al.
7,691,121	B2	4/2010	Rosenbluth	9,005,172	B2	4/2015	Chung
7,695,458	B2	4/2010	Belley et al.	9,028,401	B1	5/2015	Bacich et al.
7,763,010	B2	7/2010	Evans et al.	9,078,682	B2	7/2015	Lenker et al.
7,766,934	B2	8/2010	Pal et al.	9,101,382	B2	8/2015	Krolik et al.
7,775,501	B2*	8/2010	Kees F16K 7/065 251/5	9,125,683	B2	9/2015	Farhangnia et al.
7,780,696	B2	8/2010	Daniel et al.	9,126,016	B2	9/2015	Fulton
7,905,877	B1	3/2011	Oscar et al.	9,149,609	B2	10/2015	Ansel et al.
7,905,896	B2	3/2011	Straub	9,155,552	B2	10/2015	Ulm, III
7,938,809	B2	5/2011	Lampropoulos et al.	9,161,766	B2	10/2015	Slee et al.
7,938,820	B2	5/2011	Webster et al.	9,173,668	B2	11/2015	Ulm, III
7,967,790	B2	6/2011	Whiting et al.	9,186,487	B2	11/2015	Dubrul et al.
7,976,511	B2	7/2011	Fotjik	9,204,887	B2	12/2015	Cully et al.
7,993,302	B2	8/2011	Hebert et al.	9,216,277	B2	12/2015	Myers
7,993,363	B2	8/2011	Demond et al.	9,358,037	B2	1/2016	Farhangnia et al.
8,043,313	B2	10/2011	Krolik et al.	9,259,237	B2	2/2016	Quick et al.
8,052,640	B2	11/2011	Fiorella et al.	9,283,066	B2	3/2016	Hopkins et al.
8,057,496	B2	11/2011	Fischer, Jr.	9,351,747	B2	5/2016	Kugler et al.
8,057,497	B1	11/2011	Raju et al.	9,439,664	B2	9/2016	Sos
8,066,757	B2	11/2011	Ferrera et al.	9,439,751	B2	9/2016	White et al.
8,070,769	B2	12/2011	Broome	9,456,834	B2	10/2016	Folk
8,070,791	B2	12/2011	Ferrera et al.	9,463,035	B1	10/2016	Greenhalgh et al.
8,075,510	B2	12/2011	Aklog et al.	9,463,036	B2	10/2016	Brady et al.
8,088,140	B2	1/2012	Ferrera et al.	9,526,864	B2	12/2016	Quick
8,092,486	B2	1/2012	Berrada et al.	9,526,865	B2	12/2016	Quick
				9,566,424	B2	2/2017	Pessin
				9,579,116	B1	2/2017	Nguyen et al.
				9,616,213	B2	4/2017	Furnish et al.
				9,636,206	B2	5/2017	Nguyen et al.
				9,643,035	B2	5/2017	Mastenbroek

(56)

References Cited

U.S. PATENT DOCUMENTS

9,700,332 B2	7/2017	Marchand et al.	2003/0135230 A1	7/2003	Massey et al.
9,717,514 B2	8/2017	Martin et al.	2003/0135258 A1	7/2003	Andreas et al.
9,717,519 B2	8/2017	Rosenbluth et al.	2003/0153873 A1	8/2003	Luther et al.
9,744,024 B2	8/2017	Nguyen et al.	2003/0153973 A1	8/2003	Soun et al.
9,757,137 B2	9/2017	Krolik et al.	2003/0168068 A1	9/2003	Poole et al.
9,827,084 B2	11/2017	Bonnette et al.	2003/0176884 A1	9/2003	Berrada et al.
9,844,386 B2	12/2017	Nguyen et al.	2003/0191516 A1	10/2003	Weldon et al.
9,844,387 B2	12/2017	Marchand et al.	2003/0208224 A1	11/2003	Broome
9,848,975 B2	12/2017	Hauser	2003/0216774 A1	11/2003	Larson
9,849,014 B2	12/2017	Kusleika	2004/0039412 A1	2/2004	Isshiki et al.
9,962,178 B2	5/2018	Greenhalgh et al.	2004/0068288 A1	4/2004	Palmer et al.
9,980,813 B2*	5/2018	Eller F16K 7/06	2004/0073243 A1	4/2004	Sepetka et al.
9,999,493 B2	6/2018	Nguyen et al.	2004/0098033 A1	5/2004	Leeflang et al.
10,004,531 B2	6/2018	Rosenbluth et al.	2004/0122359 A1	6/2004	Wenz et al.
10,010,335 B2	7/2018	Greenhalgh et al.	2004/0127936 A1	7/2004	Salahieh et al.
10,016,266 B2	7/2018	Hauser	2004/0133232 A1	7/2004	Rosenbluth et al.
10,028,759 B2	7/2018	Wallace et al.	2004/0138525 A1	7/2004	Saadat et al.
10,045,790 B2	8/2018	Cox et al.	2004/0138692 A1	7/2004	Phung et al.
10,098,651 B2	10/2018	Marchand et al.	2004/0167567 A1	8/2004	Cano et al.
10,130,385 B2	11/2018	Farhangnia et al.	2004/0199201 A1	10/2004	Kellett et al.
10,226,263 B2	3/2019	Look et al.	2004/0199202 A1	10/2004	Dubrul et al.
10,238,406 B2	3/2019	Cox et al.	2004/0260344 A1	12/2004	Lyons et al.
10,271,864 B2	4/2019	Greenhalgh et al.	2004/0267272 A1	12/2004	Henniges et al.
10,327,883 B2	6/2019	Yachia	2005/0033172 A1	2/2005	Dubrul et al.
10,335,186 B2	7/2019	Rosenbluth et al.	2005/0038468 A1	2/2005	Panetta et al.
10,342,571 B2	7/2019	Marchand et al.	2005/0054995 A1	3/2005	Barzell et al.
10,349,960 B2	7/2019	Quick	2005/0055047 A1	3/2005	Greenhalgh
10,383,644 B2	8/2019	Molaei et al.	2005/0085769 A1	4/2005	MacMahon et al.
10,478,535 B2	11/2019	Ogle	2005/0085826 A1	4/2005	Nair et al.
10,524,811 B2	1/2020	Marchand et al.	2005/0085846 A1	4/2005	Carrison et al.
10,588,655 B2	3/2020	Rosenbluth et al.	2005/0085849 A1	4/2005	Sepetka et al.
10,695,159 B2	6/2020	Hauser	2005/0119668 A1	6/2005	Teague et al.
10,709,471 B2	7/2020	Rosenbluth et al.	2005/0177132 A1	8/2005	Lentz et al.
10,799,331 B2	10/2020	Hauser	2005/0187570 A1	8/2005	Nguyen et al.
10,912,577 B2	2/2021	Marchand et al.	2005/0283165 A1	12/2005	Gadberry
11,000,682 B2	5/2021	Merritt et al.	2005/0283166 A1	12/2005	Greenhalgh et al.
11,013,523 B2	5/2021	Arad Hadar	2005/0283186 A1	12/2005	Berrada et al.
11,058,445 B2	7/2021	Cox et al.	2006/0020286 A1	1/2006	Niermann
11,058,451 B2	7/2021	Marchand et al.	2006/0042786 A1	3/2006	West
11,147,571 B2	10/2021	Cox et al.	2006/0047286 A1	3/2006	West
11,154,314 B2	10/2021	Quick	2006/0074401 A1	4/2006	Ross
11,259,821 B2	3/2022	Buck et al.	2006/0089533 A1	4/2006	Ziegler et al.
11,406,801 B2	8/2022	Fojtik et al.	2006/0100662 A1	5/2006	Daniel et al.
11,433,218 B2	9/2022	Quick et al.	2006/0155305 A1	7/2006	Freudenthal et al.
11,439,799 B2	9/2022	Buck et al.	2006/0173525 A1	8/2006	Behl et al.
11,457,936 B2	10/2022	Buck et al.	2006/0195137 A1	8/2006	Sepetka et al.
11,529,158 B2	12/2022	Hauser	2006/0200221 A1	9/2006	Malewicz
11,554,005 B2	1/2023	Merritt et al.	2006/0217664 A1	9/2006	Hattier et al.
11,559,382 B2	1/2023	Merritt et al.	2006/0224177 A1	10/2006	Finitis
2001/0004699 A1	6/2001	Gittings et al.	2006/0229645 A1	10/2006	Bonnette et al.
2001/0041909 A1	11/2001	Tsugita et al.	2006/0247500 A1	11/2006	Voegele et al.
2001/0049486 A1	12/2001	Evans et al.	2006/0253145 A1	11/2006	Lucas
2001/0051810 A1	12/2001	Dubrul et al.	2006/0276874 A1	12/2006	Wilson et al.
2002/0022858 A1	2/2002	Demond et al.	2006/0282111 A1	12/2006	Morsi
2002/0022859 A1	2/2002	Hogendijk	2006/0293696 A1	12/2006	Fahey et al.
2002/0026211 A1	2/2002	Khosravi et al.	2007/0010787 A1	1/2007	Hackett et al.
2002/0032455 A1	3/2002	Boock et al.	2007/0038225 A1	2/2007	Osborne
2002/0049452 A1	4/2002	Kurz et al.	2007/0093744 A1	4/2007	Elmaieh
2002/0095161 A1	7/2002	Dhindsa	2007/0112374 A1	5/2007	Paul, Jr. et al.
2002/0095171 A1	7/2002	Belef	2007/0118165 A1	5/2007	DeMello et al.
2002/0111648 A1	8/2002	Kusleika et al.	2007/0149996 A1	6/2007	Coughlin
2002/0120277 A1	8/2002	Hauschild et al.	2007/0161963 A1	7/2007	Smalling
2002/0147458 A1	10/2002	Hiblar et al.	2007/0179513 A1	8/2007	Deutsch
2002/0151918 A1	10/2002	Lafontaine et al.	2007/0191866 A1	8/2007	Palmer et al.
2002/0156457 A1	10/2002	Fisher	2007/0198028 A1	8/2007	Miloslavski et al.
2002/0161392 A1	10/2002	Dubrul	2007/0208361 A1	9/2007	Okushi et al.
2002/0169474 A1	11/2002	Kusleika	2007/0208367 A1	9/2007	Fiorella et al.
2002/0173819 A1	11/2002	Leeflang et al.	2007/0213753 A1	9/2007	Waller
2002/0188276 A1	12/2002	Evans et al.	2007/0213765 A1	9/2007	Adams et al.
2003/0083693 A1	5/2003	Daniel et al.	2007/0255252 A1	11/2007	Mehta
2003/0100919 A1	5/2003	Hopkins et al.	2007/0288054 A1	12/2007	Tanaka et al.
2003/0114875 A1	6/2003	Sjostrom	2008/0015541 A1	1/2008	Rosenbluth et al.
2003/0116731 A1*	6/2003	Hartley F16K 7/06 251/297	2008/0088055 A1	4/2008	Ross
2003/0125663 A1	7/2003	Coleman et al.	2008/0157017 A1	7/2008	Macatangay et al.
			2008/0167678 A1	7/2008	Morsi
			2008/0183136 A1	7/2008	Lenker et al.
			2008/0228209 A1	9/2008	DeMello et al.
			2008/0234715 A1	9/2008	Pesce et al.
			2008/0234722 A1	9/2008	Bonnette et al.

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO2010023671	3/2010
WO	WO2010049121	5/2010
WO	WO2010102307	9/2010
WO	WO2011032712	3/2011
WO	WO2011054531	5/2011
WO	WO2011073176	6/2011
WO	WO2012009675	1/2012
WO	WO2012011097	1/2012
WO	WO2012049652	4/2012
WO	WO2012065748	5/2012
WO	WO2012120490	9/2012
WO	WO2012162437	11/2012
WO	WO2014047650	3/2014
WO	WO2014081892	5/2014
WO	WO2015006782	1/2015
WO	WO2015061365	4/2015
WO	WO2015121424	8/2015
WO	WO2015189354	12/2015
WO	WO2015191646	12/2015
WO	WO2017024258	2/2017
WO	WO2017058280	4/2017
WO	WO2017070702	4/2017
WO	WO2017106877	6/2017
WO	WO2017189535	11/2017
WO	WO2017189550	11/2017
WO	WO2017189591	11/2017
WO	WO2017189615	11/2017
WO	WO2017210487	12/2017
WO	WO2018049317	3/2018
WO	WO2018080590	5/2018
WO	WO2018148174	8/2018
WO	WO2019010318	1/2019
WO	WO2019050765	3/2019
WO	WO2019075444	4/2019
WO	WO2019094456	5/2019
WO	WO2019222117	11/2019
WO	WO2019246240	12/2019
WO	WO2020036809	2/2020
WO	WO2021067134	4/2021
WO	WO2021076954	4/2021
WO	WO2021127202	6/2021
WO	WO2021248042	12/2021
WO	WO2022032173	2/2022
WO	WO2022103848	5/2022
WO	WO2022109021	5/2022
WO	WO2022109034	5/2022

OTHER PUBLICATIONS

Gibbs, et al., "Temporary Stent as a bail-out device during percutaneous transluminal coronary angioplasty: preliminary clinical experience," *British Heart Journal*, 1994, 71:372-377, Oct. 12, 1993, 6 pgs.

Gupta, S. et al., "Acute Pulmonary Embolism Advances in Treatment", JAPI, Association of Physicians India, Mar. 2008, vol. 56, 185-191.

International Search Report and Written Opinion for International App. No. PCT/US13/61470, dated Jan. 17, 2014, 7 pages.

International Search Report and Written Opinion for International App. No. PCT/US2014/046567, dated Nov. 3, 2014, 13 pages.

International Search Report and Written Opinion for International App. No. PCT/US2014/061645, dated Jan. 23, 2015, 15 pages.

International Search Report for International App. No. PCT/US13/71101, dated Mar. 31, 2014, 4 pages.

Konstantinides, S. et al., "Pulmonary embolism hotline 2012—Recent and expected trials", *Thrombosis and Haemostasis*, Jan. 9, 2013:33; 43-50.

Konstantinides, S. et al., "Pulmonary embolism: risk assessment and management", *European Society of Cardiology; European Heart Journal*, Sep. 7, 2012:33, 3014-3022.

Kucher, N. et al., "Percutaneous Catheter Thrombectomy Device for Acute Pulmonary Embolism: In Vitro and in Vivo Testing", *Circulation*, Sep. 2005:112:e28-e32.

Kucher, N., "Catheter Interventions in Massive Pulmonary Embolism", *Cardiology Rounds*, Mar. 2006 vol. 10, Issue 3, 6 pages.

Kucher, N. et al., "Management of Massive Pulmonary Embolism", *Radiology*, Sep. 2005:236:3 852-858.

Kucher, N. et al., "Randomized, Controlled Trial of Ultrasound-Assisted Catheter-Directed Thrombolysis for Acute Intermediate-Risk Pulmonary Embolism." *Circulation*, 2014, 129, pp. 9 pages.

Kuo, W. et al., "Catheter-directed Therapy for the Treatment of Massive Pulmonary Embolism: Systematic Review and Meta-analysis of Modern Techniques", *Journal of Vascular and Interventional Radiology*, Nov. 2009:20:1431-1440.

Kuo, W. et al., "Catheter-Directed Embolectomy, Fragmentation, and Thrombolysis for the Treatment of Massive Pulmonary Embolism After Failure of Systemic Thrombolysis", *American College of CHEST Physicians* 2008: 134:250-254.

Kuo, W. MD, "Endovascular Therapy for Acute Pulmonary Embolism", *Continuing Medical Education Society of Interventional Radiology ("CME")*; *Journal of Vascular and Interventional Radiology*, Feb. 2012: 23:167-179.

Lee, L. et al., "Massive pulmonary embolism: review of management strategies with a focus on catheter-based techniques", *Expert Rev. Cardiovasc. Ther.* 8(6), 863-873 (2010).

Liu, S. et al., "Massive Pulmonary Embolism: Treatment with the Rotarex Thrombectomy System", *Cardiovascular Interventional Radiology*; 2011: 34:106-113.

Muller-Hulsbeck, S. et al. "Mechanical Thrombectomy of Major and Massive Pulmonary Embolism with Use of the Amplatz Thrombectomy Device", *Investigative Radiology*, Jun. 2001:36:6:317-322.

Reekers, J. et al., "Mechanical Thrombectomy for Early Treatment of Massive Pulmonary Embolism", *Cardiovascular and Interventional Radiology*, 2003: 26:246-250.

Schmitz-Rode et al., "New Mesh Basket for Percutaneous Removal of Wall-Adherent Thrombi in Dialysis Shunts," *Cardiovasc Intervent Radiol* 16:7-10 1993 4 pgs.

Schmitz-Rode et al., "Temporary Pulmonary Stent Placement as Emergency Treatment of Pulmonary Embolism," *Journal of the American College of Cardiology*, vol. 48, No. 4, 2006 (5 pgs.).

Schmitz-Rode, T. et al., "Massive Pulmonary Embolism: Percutaneous Emergency Treatment by Pigtail Rotation Catheter", *JACC Journal of the American College of Cardiology*, Aug. 2000:36:2:375-380.

Spiotta, A et al., "Evolution of thrombectomy approaches and devices for acute stroke: a technical review," *J NeuroIntervent Surg* 2015, 7, pp. 7 pages.

Svilaas, T. et al., "Thrombus Aspiration During Primary Percutaneous Coronary Intervention." *The New England Journal of Medicine*, 2008, vol. 358, No. 6, 11 pages.

Tapson, V., "Acute Pulmonary Embolism", *The New England Journal of Medicine*, Mar. 6, 2008:358:2037-52.

The Penumbra Pivotal Stroke Trial Investigators, "The Penumbra Pivotal Stroke Trial: Safety and Effectiveness of a New Generation of Mechanical Devices for Clot Removal in Intracranial Large Vessel Occlusive Disease." *Stroke*, 2009, 40: pp. 9 pages.

Truong et al., "Mechanical Thrombectomy of Iliocaval Thrombosis Using a Protective Expandable Sheath," *Cardiovasc Intervent Radiol* 27:254-258, 2004, 5 pgs.

Turk et al., "ADAPT FAST study: a direct aspiration first pass technique for acute stroke thrombectomy." *J NeuroIntervent Surg*, vol. 6, 2014, 6 pages.

Uflacker, R., "Interventional Therapy for Pulmonary Embolism", *Journal of Vascular and Interventional Radiology*, Feb. 2001: 12:147-164.

Verma, R., MD et al. "Evaluation of a Newly Developed Percutaneous Thrombectomy Basket Device in Sheep With Central Pulmonary Embolisms", *Investigative Radiology*, Oct. 2006, 41, 729-734.

International Search Report and Written Opinion for International App. No. PCT/US2015/034987 filed Jun. 9, 2015, Applicant: Inceptus Medical, LLC, dated Sep. 17, 2015, 12 pages.

English translation of Japanese Office Action received for JP Application No. 2016-564210, Applicant: Inceptus Medical, LLC, dated Sep. 4, 2017, 4 pages.

(56)

References Cited

OTHER PUBLICATIONS

Australian Exam Report received for AU Application No. 2015274704, Applicant: Inceptus Medical, LLC, dated Sep. 7, 2017, 3 pages.

European Search Report received for EP Application No. 15805810.7, Applicant: Inceptus Medical, LLC, dated Sep. 4, 2017, 6 pages.

International Search Report and Written Opinion for International App. No. PCT/US2016/067628 filed Dec. 19, 2016, Applicant: Inari Medical, Inc., dated Apr. 10, 2017, 11 pages.

Goldhaber, S. et al. "Percutaneous Mechanical Thrombectomy for Acute Pulmonary Embolism—A Double-Edged Sword," American College of CHEST Physicians, Aug. 2007, 132:2, 363-372.

Goldhaber, S., "Advanced treatment strategies for acute pulmonary embolism, including thrombolysis and embolectomy," Journal of Thrombosis and Haemostasis, 2009: 7 (Suppl. 1): 322-327.

International Search Report and Written Opinion for International App. No. PCT/US2017/029696, Date of Filing: Apr. 26, 2017, Applicant: Inari Medical, Inc., dated Sep. 15, 2017, 19 pages.

International Search Report and Written Opinion for International App. No. PCT/US2016/058536, Date of Filing: Oct. 24, 2016, Applicant: Inari Medical, Inc., dated Mar. 13, 2017, 14 pages.

European First Office Action received for EP Application No. 13838945.7, Applicant: Inari Medical, Inc., dated Oct. 26, 2018, 7 pages.

International Search Report and Written Opinion for International App. No. PCT/US2018/048786, Date of Filing: Aug. 30, 2018, Applicant: Inari Medical, Inc., dated Dec. 13, 2018, 12 pages.

International Search Report and Written Opinion for International App. No. PCT/US2018/055780, Date of Filing: Oct. 13, 2018, Applicant: Inceptus Medical LLC., dated Jan. 22, 2019, 8 pages.

European Search Report for European Application No. 16876941.2, Date of Filing: Dec. 19, 2016, Applicant: Inari Medical, Inc., dated Jul. 18, 2019, 7 pages.

Extended European Search Report for European Application No. 16858462.1, Date of Filing: Oct. 24, 2016, Applicant: Inari Medical, Inc., dated Jun. 3, 2019, 10 pages.

International Search Report and Written Opinion for International App. No. PCT/US2019/045794, Date of Filing: Aug. 8, 2019, Applicant: Inari Medical, Inc., dated Nov. 1, 2019, 17 pages.

Partial Supplementary European Search Report for European Application No. 17864818.4, Date of Filing: May 21, 2019, Applicant: Inari Medical, Inc., dated Apr. 24, 2020, 11 pages.

International Search Report and Written Opinion for International App. No. PCT/US2020/056067, Date of Filing: Oct. 16, 2020; Applicant: Inari Medical, Inc., dated Jan. 22, 2021, 8 pages.

Extended European Search Report for European Application No. 20191581.6, Applicant: Inari Medical, Inc., dated Mar. 31, 2021, 11 pages.

International Search Report and Written Opinion for International App. No. PCT/US2020/055645, Date of Filing: Dec. 17, 2020; Applicant: Inari Medical, Inc., dated Apr. 14, 2021, 12 pages.

Extended European Search Report for European Application No. 18853465.5, Applicant: Inari Medical, Inc., dated May 7, 2021, 2021, 7 pages.

Vorwerk, D. MD, et al., "Use of a Temporary Caval Filter to Assist Percutaneous Iliocaval Thrombectomy: Experimental Results." SCVIR, 1995, 4 pages.

PCT International Search Report and Written Opinion for International Appln. No. PCT/US2020/014854, dated Oct. 5, 2020 (13 pages).

PCT International Search Report and Written Opinion for International Appln. No. PCT/US2020/018655, dated Dec. 16, 2020 (22 pages).

PCT International Search Report and Written Opinion for International Appln. No. PCT/US2020/017684, dated Nov. 30, 2020 (19 pages).

Extended European Search Report for EP Patent Appln. No. 20185092.2 dated Sep. 11, 2020, 6 pages.

EP Examination Report for EP Patent Appln. No. 18745794.0 dated Jul. 20, 2020, 4 pages.

Wikipedia; Embolectomy; retrieved from the internet: <https://en.wikipedia.org/wiki/Embolectomy>; 4 pgs.; retrieved/printed: Mar. 24, 2016.

O'Sullivan; Thrombolysis versus thrombectomy in acute deep vein thrombosis; *Interventional Cardiology*; 3(5); pp. 589-596; Oct. 2011.

Capture Vascular Systems; (company website); retrieved from the internet: <http://www.capturevascular.com>; 3 pgs.; retrieved/printed: Mar. 24, 2016.

Edwards Lifesciences; Fogarty® Occlusion Catheters (product brochure); retrieved from the internet: <http://web.archive.org/web/20150228193218/http://www.edwards.com/products/vascular/atraumaticocclusion/pages/occlusioncatheter.aspx>; © 2011; 2 pgs.; retrieved/printed: Mar. 24, 2011.

Boston Scientific; Fetch(TM) 2 Aspiration Catheter (product information); retrieved from the internet: <http://www.bostonscientific.com/en-US/products/thrombectomy-systems/2-aspiration-catheter.html>; 2 pgs.; retrieved/printed: Mar. 24, 2016.

Penumbra, Inc.; Indigo® System (product information); retrieved from the internet: <http://www.penumbra.com/peripheralpercutaneous-thromboembolectomy/indigo-system>; 7 pgs.; retrieved/printed: Mar. 24, 2016.

YouTube; Merci Retrieval System X Series Animation; uploaded Mar. 16, 2009 (product information); posted on May 7, 2009 by SSMDePAUL, time 1:09, retrieved from the internet: <https://www.youtube.com/watch?v=MGX7deuFkhc>; 3 pgs.; retrieved/printed: Mar. 24, 2016.

Covidien; Solitaire(TM) AS Neurovascular Remodeling Device (product information); retrieved from the internet: <http://www.ev3.net/neuro/intl/remodeling-devices/solitaire-ab.htm>; © 2015; 2 pgs.; retrieved/printed: Mar. 24, 2016.

PCT International Search Report and Written Opinion for International Patent Appln. No. PCT/US2019/050467, Applicant Stryker Corporation, dated Dec. 18, 2019 (17 pages).

PCT International Search Report and Written Opinion for International Appln. No. PCT/US2017/029440, Applicant Stryker Corporation, dated Jul. 7, 2017.

PCT International Search Report and Written Opinion for International Appln. No. PCT/US2017/029472, Applicant Stryker Corporation, dated Jul. 7, 2017.

PCT International Search Report and Written Opinion for International Appln. No. PCT/US2017/035543, Applicant Stryker Corporation, dated Aug. 14, 2017.

PCT International Search Report and Written Opinion for International Appln. No. PCT/US2017/029366, Applicant Stryker Corporation, dated Aug. 29, 2017.

PCT International Search Report and Written Opinion for International Appln. No. PCT/US2017/050933, Applicant Stryker Corporation, forms PCT/ISA/210, 220, and 237, dated Nov. 10, 2017 (16 pages).

International search report and written opinion dated Feb. 28, 2018 for PCT/US2017/029345, Applicant Stryker Corporation 26 pages.

Extended European Search Report dated Aug. 22, 2018 for European patent appln No. 16852212.6, 6 pages.

Extended European Search Report dated Oct. 5, 2018 for European patent appln No. 18174891.4, 6 pages.

International search report and written opinion dated Nov. 14, 2018 for PCT/US2018/040937, Applicant Stryker Corporation 16 pages.

International Search Report and Written Opinion dated Mar. 28, 2019 for International Appln. No. PCT/US2018/059607.

International Search Report and Written Opinion dated May 6, 2016 for PCT/US2016/017982.

PCT International Search Report and Written Opinion for International Patent Appln. No. PCT/US2019/032601, Applicant Stryker Corporation, dated Jul. 23, 2019 (12 pages).

Extended European Search Report dated Oct. 8, 2019 for European Patent Application No. 19191925.7.

International Search Report and Written Opinion for International Patent Appln. No. PCT/US2019/050410 dated Oct. 25, 2019.

International Search Report and Written Opinion for International App. No. PCT/US21/35965, Date of Filing: Jun. 4, 2021, Applicant: Inari Medical, Inc., dated Sep. 28, 2021, 12 pages.

(56)

References Cited

OTHER PUBLICATIONS

International Search Report and Written Opinion for International App. No. PCT/US21/45072 Date of Filing: Aug. 6, 2021, Applicant: Inari Medical, Inc., dated Jan. 20, 2022, 10 pages.

International Search Report and Written Opinion for International App. No. PCT/US21/58793; Date of Filing: Nov. 10, 2021, Applicant: Inari Medical, Inc., dated Mar. 16, 2022, 13 pages.

International Search Report and Written Opinion for International App. No. PCT/US21/59718; Date of Filing: Nov. 17, 2021, Applicant: Inari Medical, Inc., dated Mar. 22, 2022, 13 pages.

International Search Report and Written Opinion for International App. No. PCT/US21/59735; Date of Filing: Nov. 17, 2021, Applicant: Inari Medical, Inc., dated Mar. 22, 2022, 11 pages.

* cited by examiner

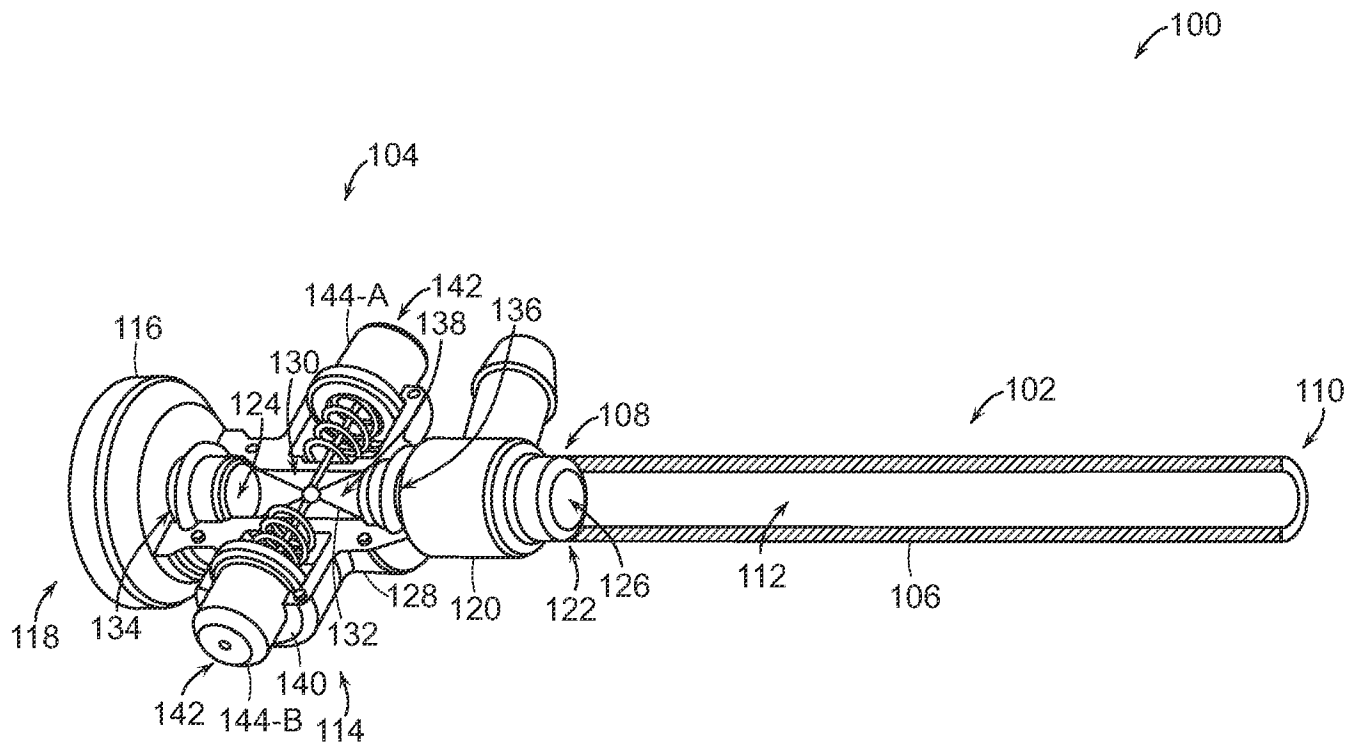


FIG. 1

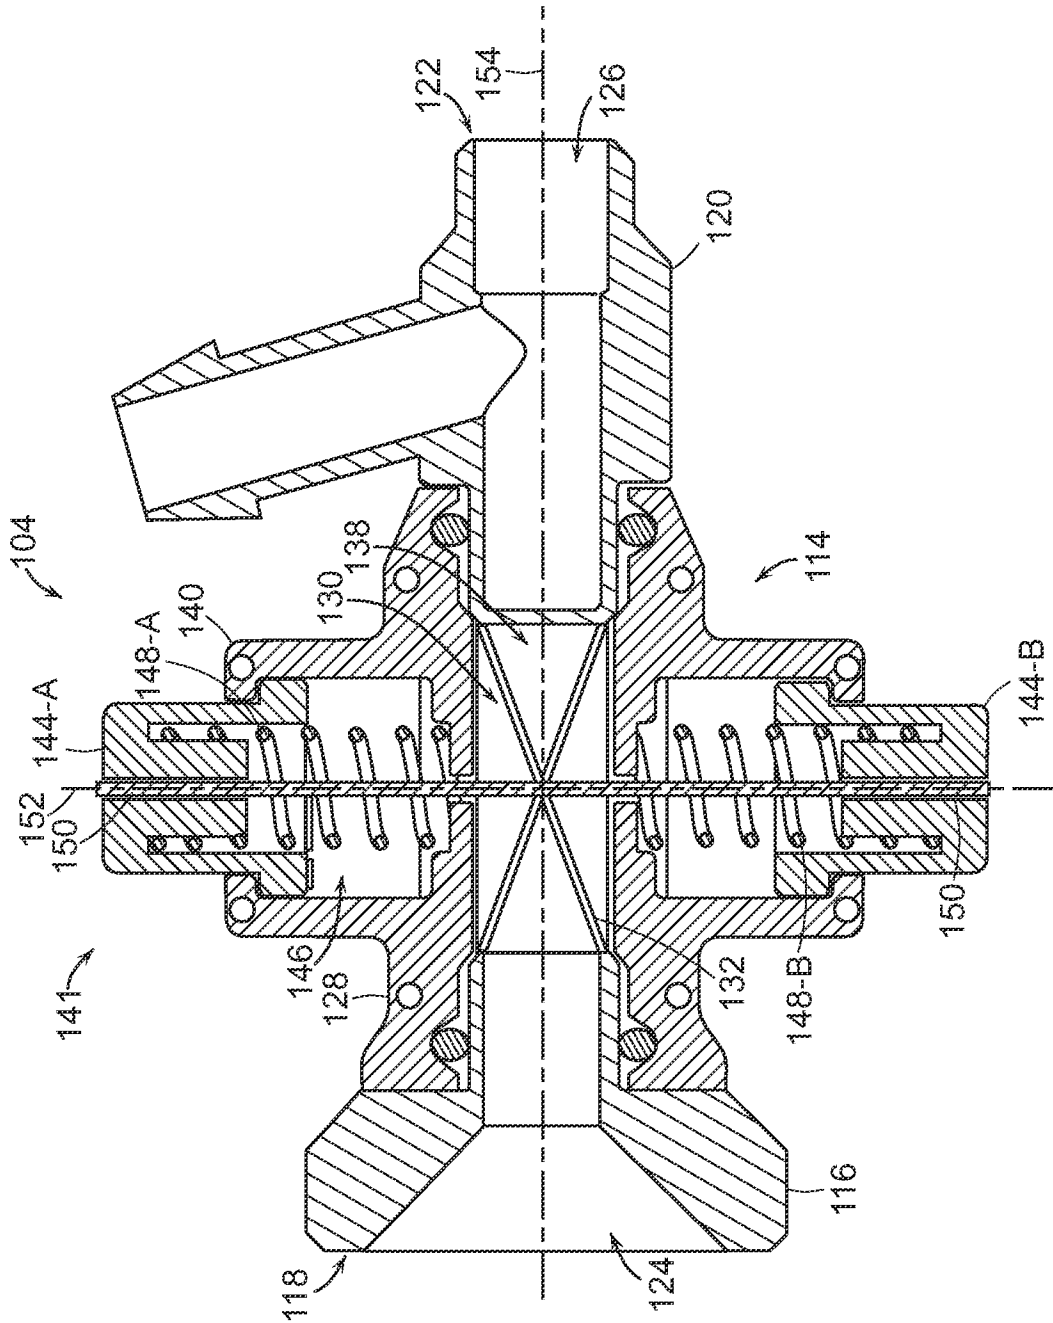
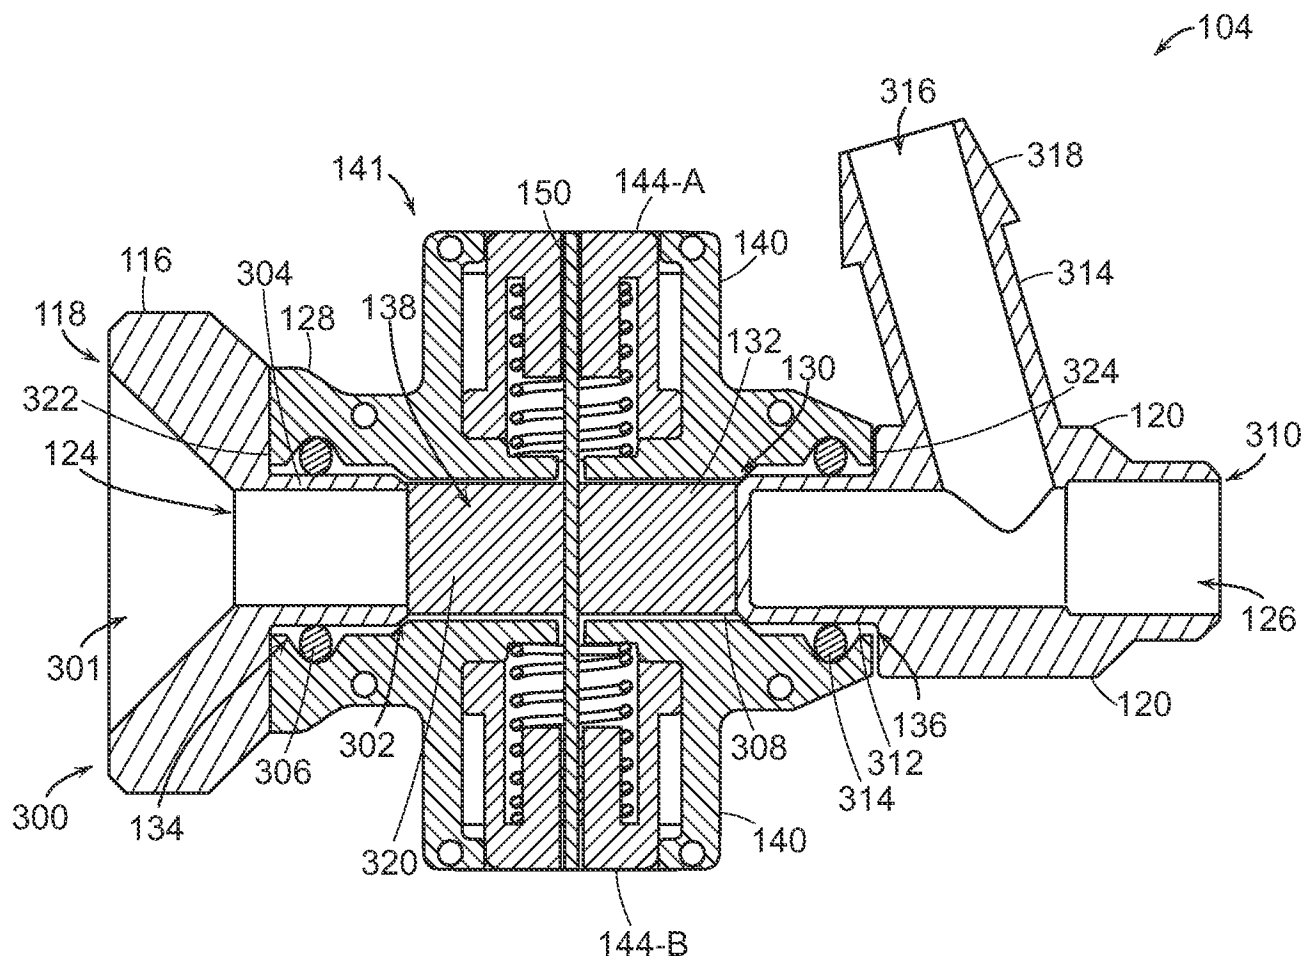


FIG. 2



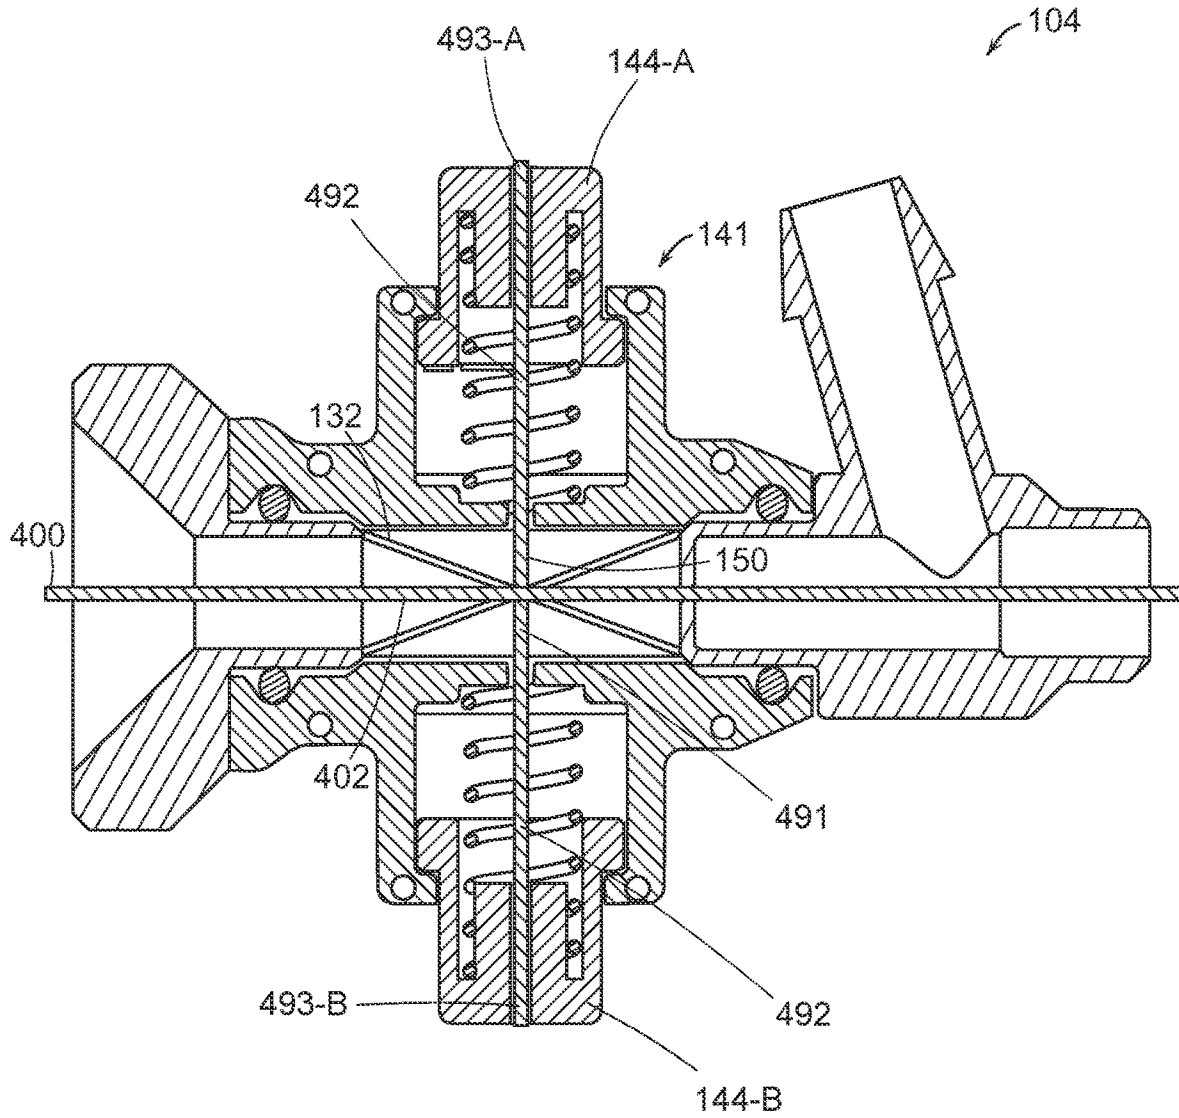


FIG. 4

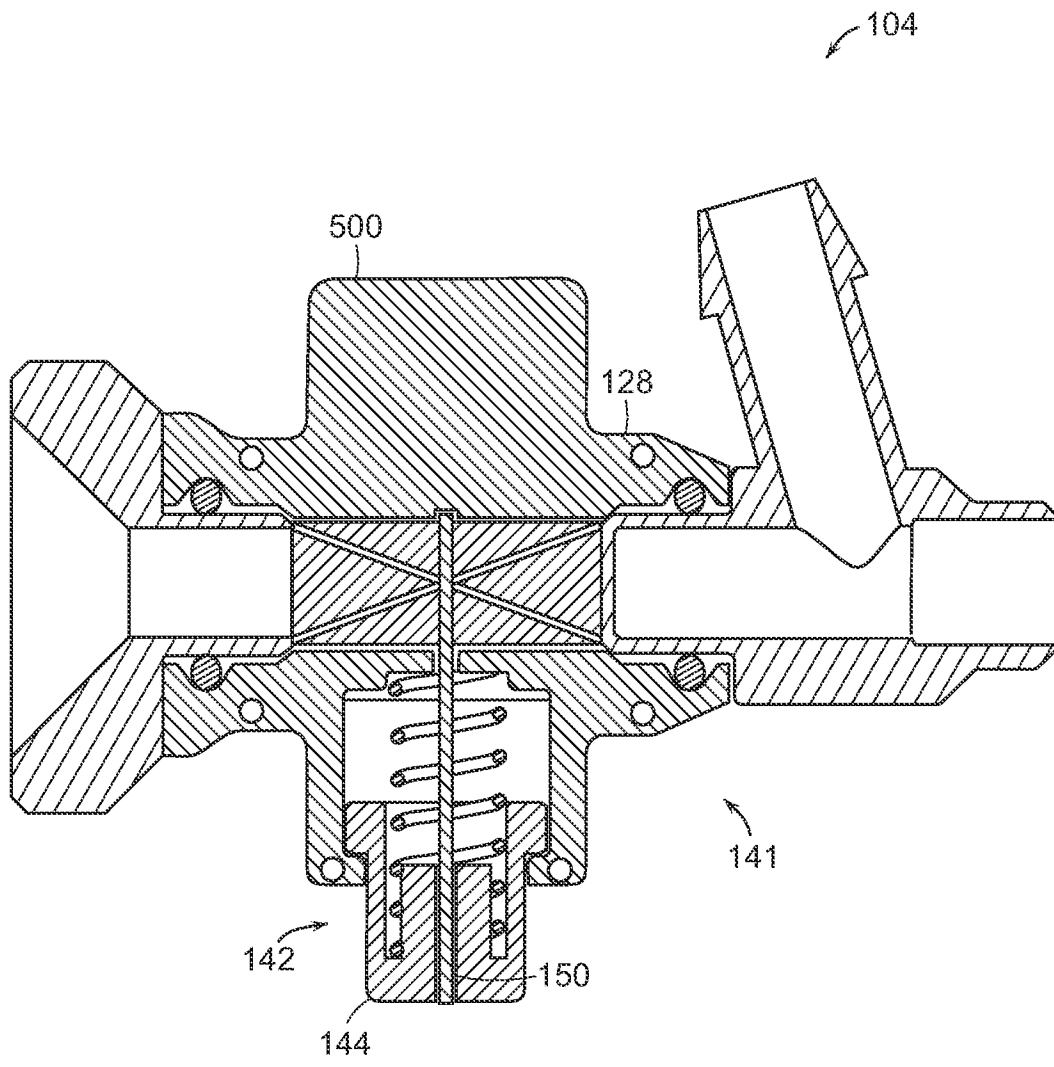


FIG. 5

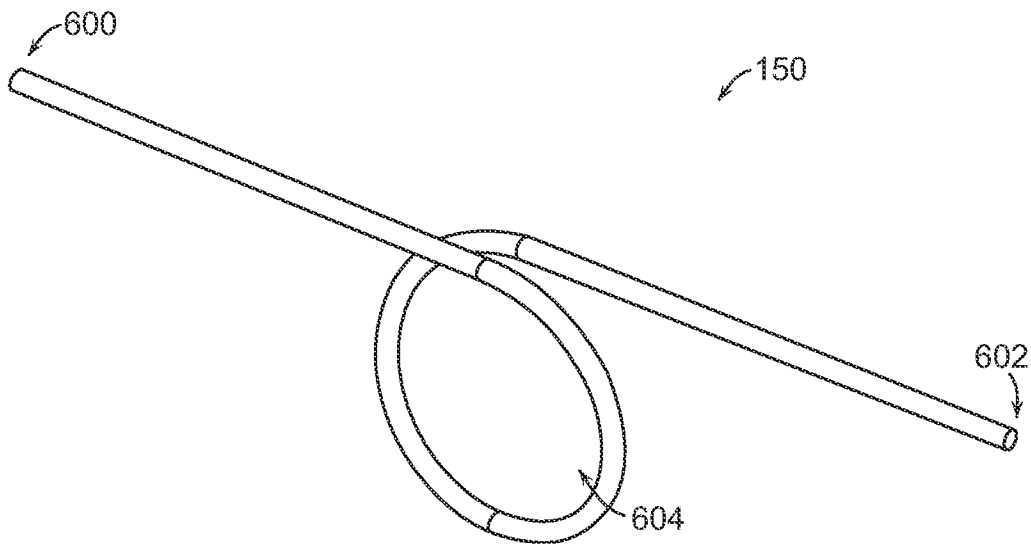


FIG. 6

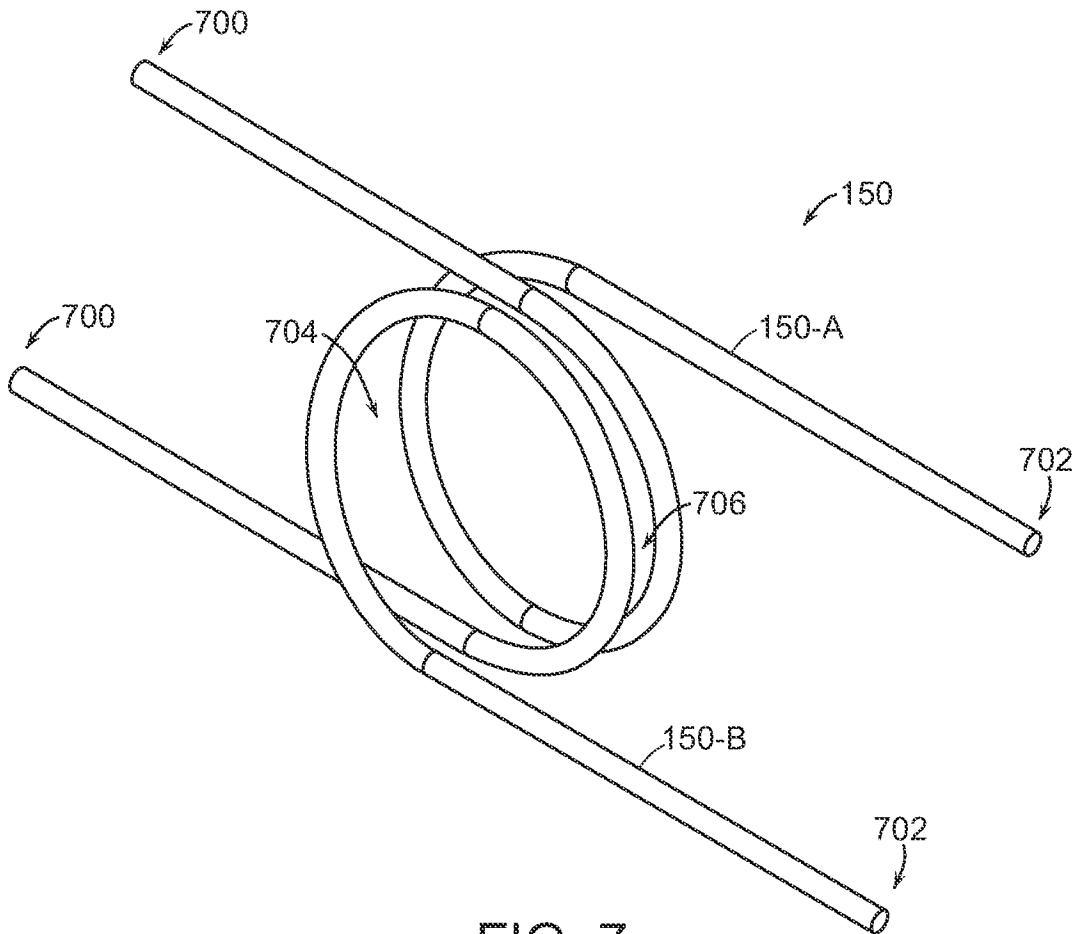


FIG. 7

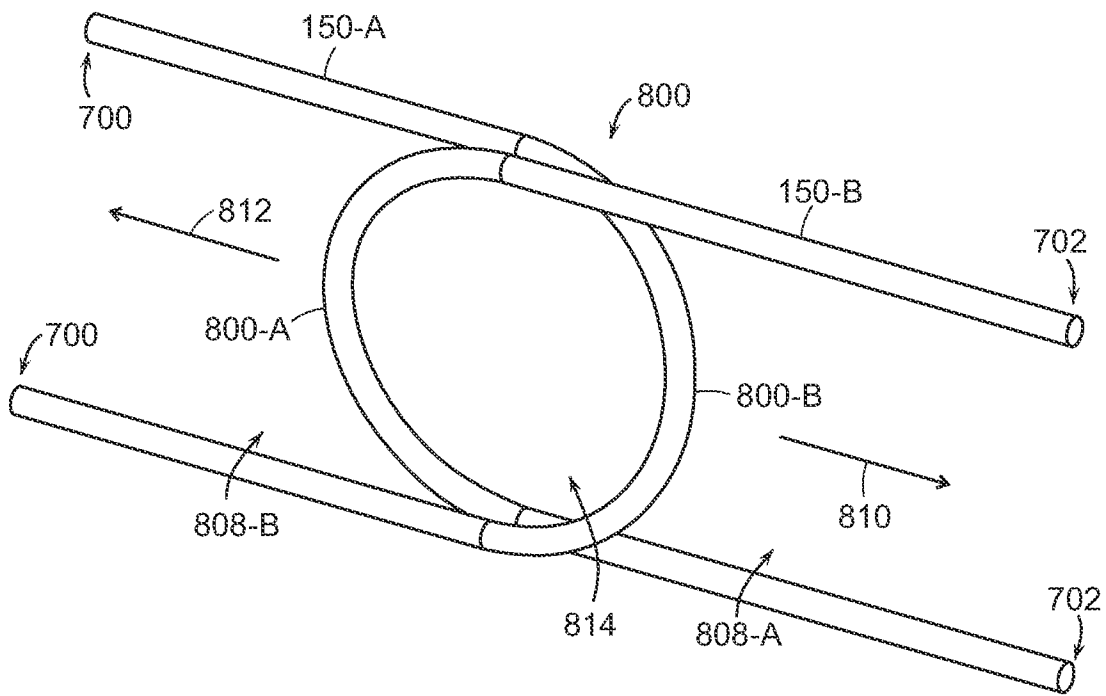


FIG. 8

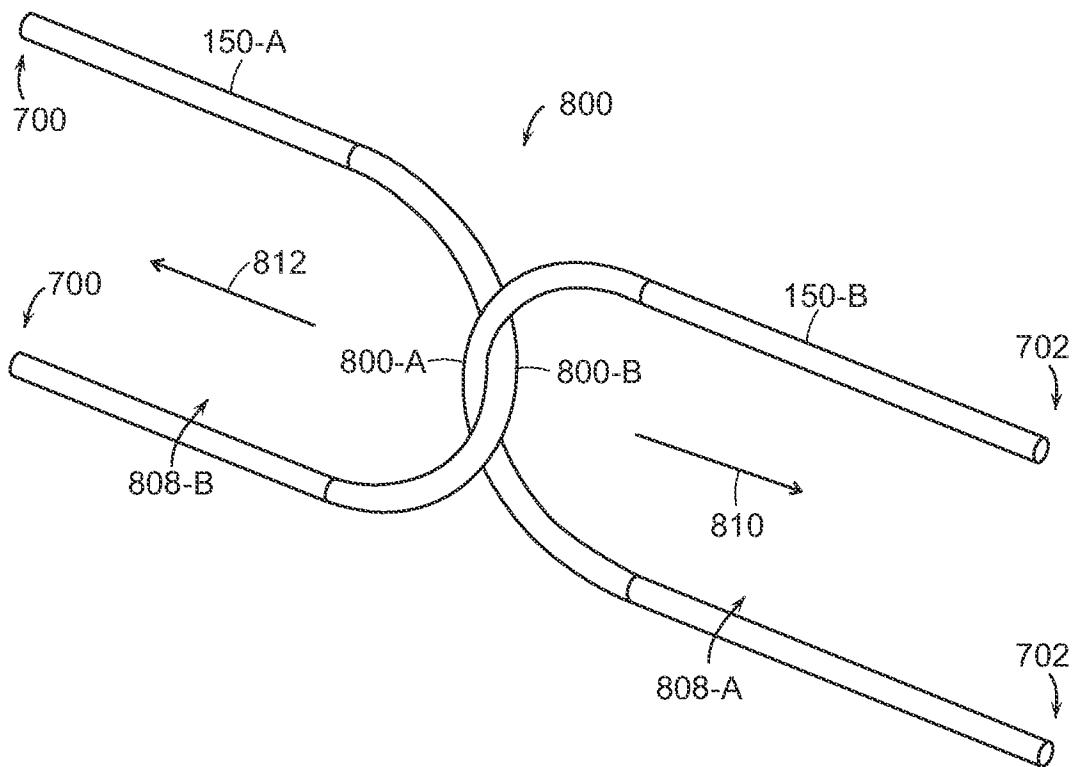


FIG. 9

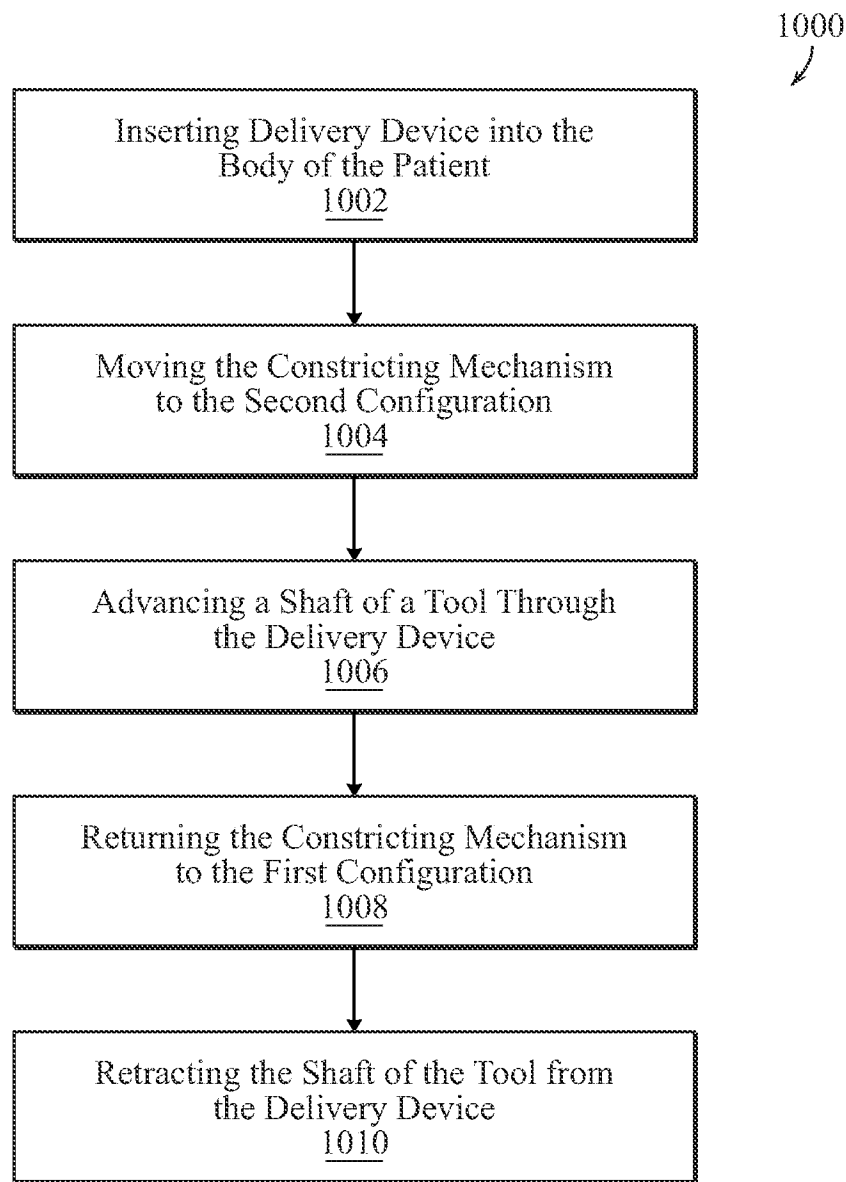


FIG. 10

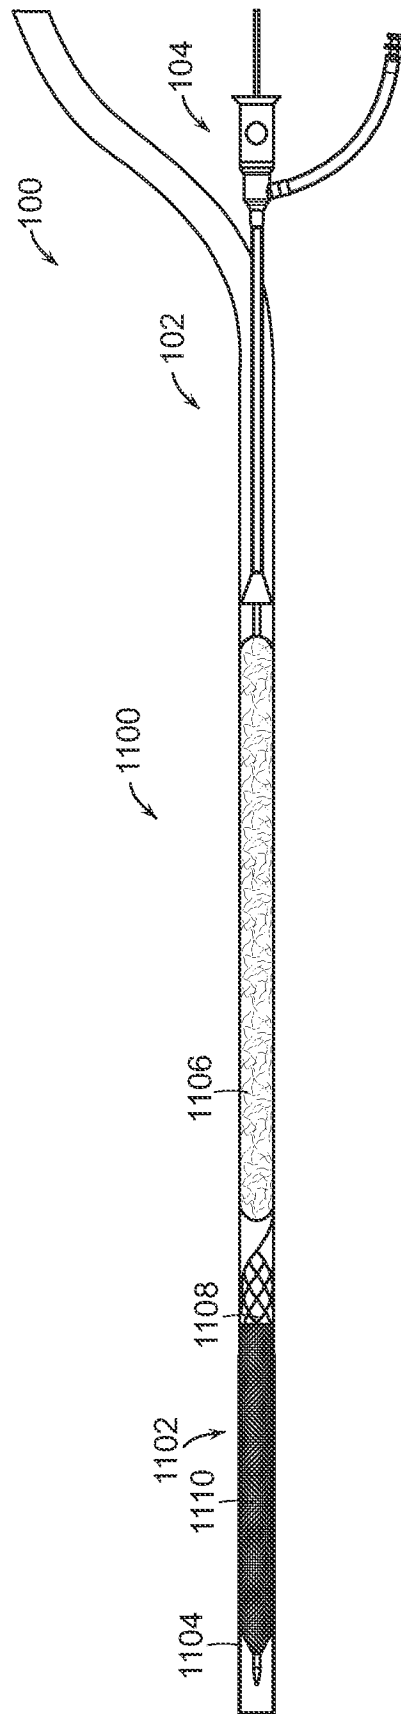


FIG. 11

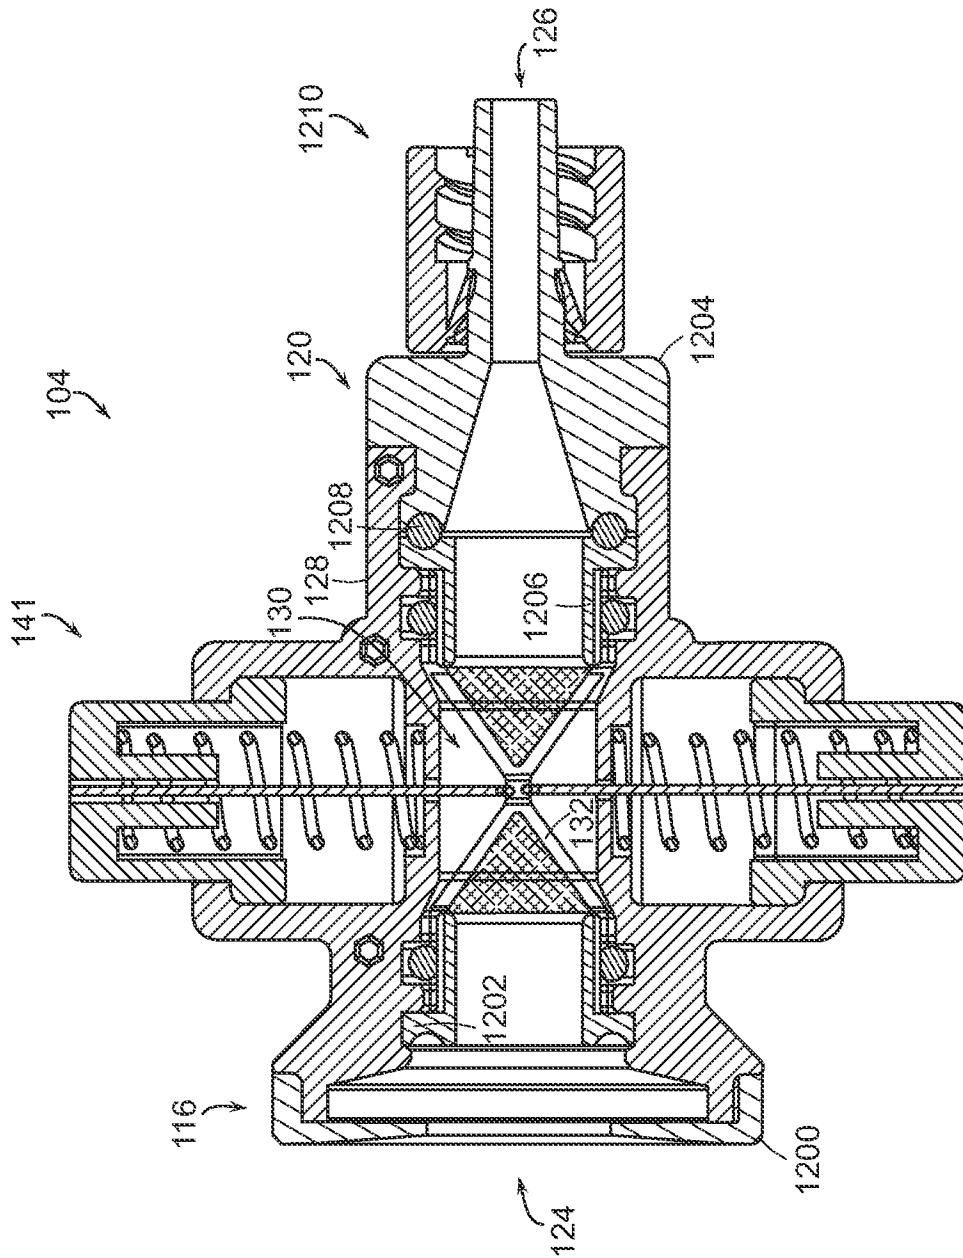


FIG. 12

1

HEMOSTASIS VALVES AND METHODS OF USE**CROSS-REFERENCE TO RELATED APPLICATIONS**

This application is a continuation of U.S. patent application Ser. No. 17/226,318, filed on Apr. 9, 2021, entitled "HEMOSTASIS VALVES AND METHODS OF USE," which is a continuation of U.S. patent application Ser. No. 16/117,519, filed on Aug. 30, 2018, now issued as U.S. Pat. No. 11,000,682, and entitled "HEMOSTASIS VALVES AND METHODS OF USE," which claims the benefit of U.S. Provisional Patent Application No. 62/554,931, filed on Sep. 6, 2017, and entitled "HEMOSTASIS VALVES AND METHODS OF USE," each of which is herein incorporated by reference in its entirety.

BACKGROUND

During a surgical procedure, a portion of a patient's body (e.g., vasculature) is accessed to allow for performance of a desired intervention or treatment. During such surgical procedures, it is desired to minimize patient blood loss, prevent delivery of air into the vasculature, and to maintain the sterility of the accessed portions or sites of the patient's body so as to prevent issues such as infection. Further, the desire for improved patient outcomes has led to the development of hemostasis valves that facilitate minimally invasive surgery.

In minimally invasive surgery, small incisions are created through a blood vessel which one or several catheters are inserted. Each of these one or several catheters can define a lumen extending longitudinally through that catheter. These catheters are moved to a position proximate to tissue, nerves, or other body structures targeted by the surgery, and then tools for performing the procedure are inserted through the lumens of some or all of these catheters.

To minimize blood loss, prevent delivery of air into the vasculature, and to facilitate maintenance of sterility within the patient's body (e.g., blood vessel), these catheters are equipped with hemostasis valves. These valves seal or selectively seal the lumens of the catheters. In many instances, these valves can seal the lumen of the catheter when a tool extends through the catheter, and specifically through the valve. Additionally the valves can seal the lumen when a tool is removed or does not extend through the catheter.

While such traditional hemostasis valves are greatly beneficial for intravascular access, they have some drawbacks. For example, some valves may not seal adequately for all interventional applications or tools, and/or the operation of some valves may be complicated for operator use. The drawbacks of such valve designs may in turn increase the complexity of any surgery performed therewith and/or reduce patient safety (e.g., bleeding, infection, and/or other detrimental complications). Accordingly, new and improved hemostasis valves and methods of use are desired.

SUMMARY

The following relates to valves, medical systems incorporating valves, and methods of using the same. The valve can include a tubular member that can be constricted, collapsed, and/or sealed by one or several tensioning mechanisms. The tensioning mechanism can include at least one filament that extends around at least a portion of the tubular member. The filament can interact with the tubular member

2

to constrict, collapse, and/or seal the tubular member via manipulation of the tensioning mechanism(s). A tool can be inserted through the valve to gain access to a patient's body and specifically to gain access to a blood vessel. Through the use of the tensioning mechanism and filament to constrict, collapse, and/or seal the tubular member, the valve can seal around a wide range of tool sizes and shapes, as well as multiple tools of differing sizes simultaneously. Additionally, such a valve creates a robust seal that maintains its seal when a vacuum is applied such as occurs during aspiration.

Aspects of the present disclosure relate to a hemostatic valve for sealing a medical device. The hemostatic valve includes an elongate member having a first end, a second end, and a central lumen extending therebetween. In some embodiments, the elongate member is pliable. The hemostatic valve can include a reinforcement structure extending along at least a portion of the elongate member, such that the reinforcement structure is coupled to the elongate member. The hemostatic valve includes an active tensioning mechanism coupled to the elongate member. In some embodiments, the tensioning mechanism is moveable between a first configuration in which the central lumen is constricted and sealed and a second configuration in which the central lumen is open. Optionally, the valve may be manually adjusted by the user to intermediate positions between fully open and fully closed. Additionally, an instrument (e.g. catheter) may provide an intermediate position where the valve creates hemostasis without user adjustment.

In some embodiments, the elongate member can be a compliant polymer tube. In some embodiments, the tensioning mechanism can include at least one filament extending at least partially around the elongate member. In some embodiments, the reinforcement structure is positioned between the at least one filament and the elongate member. In some embodiments, the reinforcement structure can be a braided mesh. In some embodiments, the reinforcement structure is coupled to the elongate member at a position proximate to the first end of the elongate member and at a position proximate to the second end of the elongate member. In some embodiments, the reinforcement structure is not coupled to the elongate member at a position between the first end of the elongate member and the second end of the elongate member. In some embodiments, the central portion of the compliant polymer tube that is constrained or collapsed by the tensioning mechanism, and at least one filament, is not coupled to the reinforcement structure.

In some embodiments, the tensioning mechanism can include an actuator coupled to the at least one filament. In some embodiments there are two tensioning mechanisms coupled to the at least one filament that operate in opposite directions. In some embodiments the two tensioning mechanisms are attached to the same filament. In some embodiments the two tensioning mechanisms are attached to opposing filaments. In some embodiments, the actuator can be moveable to control movement of the at least one filament from a first position in which the central lumen is constricted and sealed to a second position in which the central lumen is open. In some embodiments, the at least one filament is in the first position when the tensioning mechanism is in the first configuration. In some embodiments, the actuator is biased towards the first position. In some embodiments, the actuator is biased toward the second position. In some embodiments, the actuator can be a manual actuator.

In some embodiments, the at least one filament forms a loop around the elongate member. In some embodiments, the at least one filament forms a bight around a portion of the elongate member. In some embodiments, the at least one

3

filament can include a first filament and a second filament. In some embodiments, each of the first filament and the second filament are coupled to the same actuator. In some embodiments, each of the first filament and the second filament are coupled to different actuators. In some embodiments, the first filament and the second filament are moveable from the first position to the second position. In some embodiments, each of the first filament and the second filament form a loop around the elongate member. In some embodiments, the first filament forms a first bight around a first portion of the elongate member, and the second filament forms a second bight around a second portion of the elongate member. In some embodiments, the first bight extends through the second bight.

In some embodiments, the hemostatic valve can include a shell defining a first aperture and a second aperture. In some embodiments, the elongate member extends from the first aperture to the second aperture and fluidly couples the first aperture and the second aperture. In some embodiments, the tensioning mechanism is self-adjustable to seal around tools of different sizes extending through the hemostatic valve. In some embodiments, the central lumen can comprise a single lumen, and in some embodiments, the central lumen can comprise a plurality of lumens.

One aspect of the present disclosure relates to a delivery system for intravascular access of a blood vessel within a patient's body. The delivery system includes a catheter having a first end, a second end, and a catheter lumen extending therebetween and a hemostatic valve coupled to the first end of the catheter. The hemostatic valve includes a tubular member having a first end, a second end, and a central lumen extending therebetween. In some embodiments, the central lumen of the tubular member is fluidly coupled with the catheter lumen. The hemostatic valve includes an active tensioning mechanism coupled to the tubular member, the tensioning mechanism can be moveable between a first configuration in which the tensioning mechanism constricts on the central lumen and the central lumen is sealed and a second configuration in which the central lumen is open.

In some embodiments, the hemostatic valve further includes a reinforcement structure extending along at least a portion of the tubular member. In some embodiments, the reinforcement structure is located between the tensioning mechanism and the tubular member. In some embodiments, the reinforcement structure can be a braided mesh. In some embodiments, the reinforcement structure is coupled to the tubular member at a position proximate to the first end of the tubular member and at a position proximate to the second end of the tubular member. In some embodiments, the reinforcement structure is adhered to the tubular member at the first end of the tubular member and at the second end of the tubular member. In some embodiments, the reinforcement structure is uncoupled to the tubular member between the first end of the tubular member and the second end of the tubular member.

In some embodiments, the tensioning mechanism can include at least one filament extending at least partially around the tubular member. In some embodiments, the tensioning mechanism can include an actuator coupled to the at least one filament. In some embodiments, moving the tensioning mechanism from the first configuration to the second configuration can include moving the actuator and the thereto coupled at least one filament from a first position to a second position. In some embodiments, the filament constricts and seals the central lumen of the tubular member when the filament is in the first position.

4

In some embodiments, the actuator can be a manual actuator. In some embodiments, the actuator can include a pair of opposing and depressible buttons, which buttons can be biased towards an undepressed position. In some embodiments, the central lumen is sealed when the buttons are in the undepressed position. In some embodiments, the filament can be a monofilament. In some embodiments, the filament can be at least one of: a polymer filament; or a metallic filament. In some embodiments, the catheter can include a thrombus extraction device.

One aspect of the present disclosure relates to a method of sealing a delivery device accessing a blood vessel of a patient. The method includes inserting the delivery device including a catheter and a hemostatic valve into the blood vessel of the patient. In some embodiments, the catheter can have a first end, a second end, and a catheter lumen extending therethrough. In some embodiments, the hemostatic valve can be coupled to the first end and can have a tubular member defining a central lumen fluidly coupled with the catheter lumen and a tensioning mechanism coupled with the tubular member. In some embodiments, the tensioning mechanism collapses and seals the central lumen in a first configuration and thereby seals access to the blood vessel. The method can include moving the tensioning mechanism of the hemostatic valve to a second configuration. In some embodiments, the central lumen is open and access to the blood vessel is unsealed when the tensioning mechanism is in the second configuration. The method can include advancing a shaft of a tool through the delivery device until a first end of the tool reaches a desired position within the blood vessel of the patient and a portion of the shaft is positioned within the central lumen of the tubular member. The method can include returning the tensioning mechanism of the hemostatic valve to the first configuration such that the tubular member collapses on the shaft of the tool and seals around the shaft of the tool.

In some embodiments, the method includes retracting the shaft of the tool from the delivery device. In some embodiments, the tensioning mechanism is maintained in the first configuration during and after the retracting of the shaft of the tool from the delivery device. In some embodiments, the tensioning mechanism is moved to the second configuration during the retracting of the shaft of the tool from the delivery device, and the tensioning mechanism is returned to the first configuration after the shaft of the tool is retracted from the delivery device.

In some embodiments, the tensioning mechanism can include at least one filament extending at least partially around the tubular member. In some embodiments, the at least one filament collapses the tubular member when the tensioning mechanism is in the first configuration. In some embodiments, the at least one filament circumferentially constricts the tubular member to collapse the tubular member when the tensioning mechanism is in the first configuration. In some embodiments, the hemostatic valve can include a reinforcement structure located between the at least one filament and the tubular member.

In some embodiments, the at least one filament forms a loop around the elongate member, and moving the tensioning mechanism from the second configuration to the first configuration reduces a size of the loop to thereby constrict the tubular member within the loop. In some embodiments, the filament forms at least one bight around a portion of the elongate member. In some embodiments, the filament can include a first filament and a second filament. In some embodiments, the at least one bight can include a first bight oriented in a first direction and formed by the first filament

5

and a second bight oriented in a second direction and formed by the second filament. In some embodiments, the first and second bights overlap to encircle a portion of the tubular member within a constricting area.

In some embodiments, moving the tensioning mechanism from the second configuration to the first configuration can include moving the first bight in the first direction and the second bight in the direction to reduce the size of the constricting area and collapse and seal the central lumen of the tubular member. In some embodiments, the tensioning mechanism can include an actuator. In some embodiments, moving the tensioning mechanism to the second configuration can include manipulating the actuator. In some embodiments, the method includes applying a vacuum to the delivery device and/or delivery system to aspirate material through the catheter. In some embodiments, the central lumen remains sealed during the aspiration. In some embodiments, the tool can include a thrombus extraction device.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of one embodiment of a delivery device.

FIG. 2 is a side-section view of one embodiment of a hemostasis valve in a first configuration.

FIG. 3 is a side-section view of one embodiment of the valve in a second configuration.

FIG. 4 is a side-section view of one embodiment of the valve in the first configuration and with a tool extending through the valve.

FIG. 5 is a side-section view of one embodiment of a single-button hemostasis valve in a first configuration.

FIG. 6 is a perspective view of a filament of a valve forming a loop.

FIG. 7 is a perspective view of two filaments of a valve, each of the filaments forming a loop.

FIG. 8 is a perspective view of two overlapping and interlocked bights in an open configuration.

FIG. 9 is a perspective view of two overlapping and interlocked bights in a closed configuration.

FIG. 10 is a flowchart illustrating one embodiment of a method for sealing a valve and/or catheter.

FIG. 11 is a side view of one embodiment of a thrombectomy system including the delivery device.

FIG. 12 is a side-section view of another embodiment of a hemostasis valve having two-piece caps.

DETAILED DESCRIPTION

The present disclosure relates to a valve that can be used as a hemostasis valve. This valve, also referred to herein as a garrote valve can seal with or without a tool extending through the valve. The garrote valve provides convenient, single-handed operation for a wide range of medical devices including catheters, wires, embolectomy systems, or the like. This single-handed operation of the garrote valve allows the user to easily and quickly swap different tools being used through the valve without compromising hemostasis and therefore simplifying the procedure. Combined with single-handed operation, the garrote valve provides robust sealing either with or without a tool extending through the valve. This robust sealing minimizes leakage in applications with a pressure differential on different sides of the valve. This pressure differential can arise, for example, during the application of vacuum aspiration in a procedure. Even under such conditions, as well as under other condi-

6

tions, the garrote valve maintains seal integrity and prevents leakage in one or both directions.

The garrote valve includes a tubular member. The tubular member is a flexible member that defines a central lumen, which can, in some embodiments, define a single lumen, and in some embodiments, defines a plurality of lumens. In some embodiments, each of the plurality of lumens can comprise the same size and shape, and in some embodiments, some or all of the plurality of lumens can comprise different sizes and shapes. In some embodiments, for example, the plurality of lumens can comprise a lumen sized and/or shaped to receive a guide wire and a lumen sized and/or shaped to receive a tool. The tubular member extends at least partially through a constricting mechanism. The constricting mechanism can be moved from a first configuration to a second configuration, and the constricting mechanism can collapse and/or seal the central lumen of the tubular member when the constricting mechanism is in the first configuration. The constricting mechanism creates the above-discussed robust seal of the tubular member and thus of the valve.

With reference now to FIG. 1, a perspective view of one embodiment of a delivery system **100**, also referred to herein as a delivery device **100**, is shown. The delivery system **100** can include a catheter **102** and a garrote valve **104**, also referred to herein as valve **104**. The catheter **102** can comprise a shaft **106**, also referred to herein as an elongate sheath **106**, having a proximal end **108**, also referred to herein as a first end **108**, that can connect to the valve **104** and a distal end **110**, also referred to herein as a second end **110**. The shaft **106** can define a catheter lumen **112** extending from the proximal end **108** of the shaft **106** to the distal end **110** of the shaft **106**. The catheter **102** and specifically the shaft **106** can comprise a variety of shapes and sizes and can be made from a variety of materials. In some embodiments, the catheter **102** can be flexible and/or can be made from a biocompatible material. The elongate sheath **106** can have an outer diameter of at least 4 French, at least 6 French, at least 8 French, at least 10 French, at least 12 French, at least 14 French, at least 18 French, at least 20 French, at least 22 French, between 4 French and 30 French, between 8 French and 24 French, between 12 French and 20 French, and/or any other or intermediate size.

The valve **104** can include an outer shell **114**. The outer shell **114** can comprise a variety of shapes and sizes and can be made from a variety of materials. In some embodiments, the outer shell **114** can be made from one or several polymers or composites. The outer shell **114** can include features that allow interaction with and/or control of the valve **104** to move the valve **104** between the first configuration and the second configuration.

The outer shell **114** can include a proximal cap **116** located at a proximal end **118** of the outer shell **114** and a distal cap **120** located at a distal end **122** of the shell **114**. The proximal cap **116** can include and/or house a proximal aperture **124**, also referred to herein as a proximal channel **124**, a first channel **124**, or a first aperture **124**, that extends through the proximal cap **116**, and the distal cap **120** can include and/or house a distal aperture **126**, also referred to herein as a distal channel **126**, a second channel **126**, or second aperture **126**, that extends through the distal cap **120**. As seen in FIG. 1, the distal cap **120** connects to the shaft **106** of the catheter **102** at the distal end **122** of the valve **104**.

The proximal cap **116** and the distal cap **120** are connected via a housing **128**. The housing **128** can be a one-piece housing **128** or a multi-piece housing **128**. In the embodiment depicted in FIG. 1, the housing comprises a two-piece housing **128**. The housing **128** can be configured to receive

and couple with each of the proximal cap 116 and the distal cap 120, and as seen in FIG. 1, the housing 128 is coupled with each of the proximal cap 116 and the distal cap 120 to secure the relative position of the proximal cap 116 and the distal cap 120 with respect to each other.

The housing 128 can define an interior channel 130 through which an elongate member 132, also referred to herein as a tubular member 132, a septum 132, or a tubular septum 132, can extend and connect the proximal cap 116 and the distal cap 120. The elongate member 132 can comprise a variety of shapes and sizes and can be made from a variety of materials. In some embodiments, the elongate member 132 can comprise a compliant tubular structure that can be, for example, a thin-walled compliant tubular structure. The thin-walled structure of the elongate member 132 can facilitate the collapse, and specifically the uniform collapse of the elongate member 132 and the sealing of the elongate member 132. In some embodiments, the elongate member 132 is an elastic, resilient material that may comprise a polymer including either a natural or synthetic polymer. In some embodiments, the elongate member can comprise an elastic, resilient material that may comprise silicone, urethane, ethylene-vinyl acetate, natural or synthetic rubber or other elastomers known in the art. In some embodiments, the elongate member 132 can comprise a silicone tube.

The elongate member 132 can comprise a proximal end 134, also referred to herein as a first end 134, that can couple to the proximal cap 116, and a distal end 136, also referred to herein as a second end 136, that can couple to the distal cap 120. The elongate member 132 can define a central lumen 138 that can extend from the first end 134 to the second end 136 of the elongate member 132. The elongate member 132 can be coupled to the proximal cap 116 such that the central lumen 138 is fluidly coupled with the proximal aperture 124 of the proximal cap 116, and the elongate member 132 can be coupled to the distal cap 120 such that the central lumen 138, as seen in FIG. 2 and in FIG. 3, is fluidly coupled with the distal aperture 126 of the distal cap 120.

The central lumen 138 of the elongate member 132 can be defined by a wall of the elongate member 132 that can have a thickness that is uniform along the length of the elongate member 132 between the first end 134 and the second end 136, or that is non-uniform along the length of the elongate member 132 between the first end 134 and the second end 136. In some embodiments, the wall can have a thickness that is approximately between 0.005 inches and 0.05 inches, and/or approximately between 0.010 inches and 0.030 inches. As used anywhere herein, "approximately" refers to a range of +/-10% of the value and/or range of values for which "approximately" is used.

In some embodiments, the elongate member 132 can be cylindrically shaped, and specifically can be circular-cylindrically shaped. In some embodiments, the elongate member 132 can be dog-bone shaped to facilitate, for example, connection to each of the proximal cap 116 and the distal cap 120. In some embodiments, the elongate member 132 can include one or several outward-extending protuberances that engage with all or portions of a constricting mechanism 141, also referred to herein as a tensioning mechanism 141, of the valve 104 to secure a position of all or portions of the constricting mechanism 141 with respect to the elongate member 132. In some embodiments, the constricting mechanism 141 can be self-adjusting to seal around tools of different sizes extending through the valve 104.

The constricting mechanism 141 can, in some embodiments, collapse and seal the elongate member 132 via compression and/or constriction, and specifically via constriction with at least one filament 150. The constricting mechanism 141 can comprise: an actuator 142 which can be a manual actuator such as one or several buttons 144; and the at least one filament 150 that can extend at least partially around the elongate member 132. In some embodiments, the use of the constricting mechanism 141 can facilitate sealing of the valve around tools or instruments of a wide range of sizes and/or diameters, and particularly around tools or instruments that fit through the elongate member 132.

The housing 128 can further include one or several retention features 140. The one or several retention features 140 of the housing can engage with and retain all or portions of the constricting mechanism 141 of the valve 104. In some embodiments, the one or several retention features 140 of the housing 128 can retain the actuator 142 and/or can couple the actuator 142 to the housing 128. The actuator 142 can comprise any desired type of actuator including, for example, a manual actuator and/or an automated actuator such as, for example, an electromechanical actuator including a solenoid-based actuator. In some embodiments, the actuator can comprise one or several buttons 144, and specifically, as depicted in FIG. 1, the actuator 142 can comprise a first button 144-A and a second button 144-B. Alternatively, and as depicted in FIG. 5, the actuator 142 can comprise a single button 144. In such an embodiment, the filament 150 can be coupled to the single button 144 and to a portion of the housing 128 such as, for example, to grip portion 500 of the housing 128 such that the movement of the single button 144 causes the sealing and/or opening of the elongate member 132 and of the valve 104.

The actuator 142 can be biased towards a configuration such as, for example, biased towards the first configuration or biased towards the second configuration. As depicted in FIG. 2, which shows the constricting mechanism 141 in the first configuration, the actuator 142 can be biased towards the first configuration wherein the elongate member 132 is collapsed and/or sealed by a bias feature 146. In this first configuration, the buttons 144 can be in a first position, also referred to herein as an undepressed position. This bias feature 146 can, as shown in FIG. 2, include a first spring 148-A configured to bias the first button 144-A towards the first position corresponding to the first configuration of the constricting mechanism 141, and a second spring 148-B configured to bias the second button 144-B towards a first position corresponding to the first configuration of the constricting mechanism 141. One or both of the first spring 148-A and the second spring 148-B can comprise a tension spring, compression spring, a torsion spring, a coil spring, or any other desired type of spring.

In some embodiments, one or both of the first spring 148-A and the second spring 148-B can generate sufficient force so as to allow actuation of the actuator 142 with a single hand and so as to collapse and seal the elongate member 132 when the constricting mechanism 141 is in the first configuration. In some embodiments, one or both of the first spring 148-A and the second spring 148-B can generate a force of: at least 0.1 pounds, at least 0.2 pounds, at least 0.3 pounds, at least 0.4 pounds, at least 0.5 pounds, at least 0.6 pounds, at least 0.7 pounds, at least 0.8 pounds, at least 0.9 pounds, at least 1 pound, at least 1.5 pounds, at least 2 pounds, at least 3 pounds, at least 5 pounds, and/or at least 10 pounds and in some embodiments one or both of the first spring 148-A and the second spring 148-B can generate a

force approximately between: 0.1 and 10 pounds, 0.1 and 5 pounds, 0.1 and 1.5 pounds, 0.2 and 1 pounds, and/or 0.4 and 0.8 pounds.

The constricting mechanism 141 can include at least one filament 150 that extends at least partially around the elongate member 132. In some embodiments, the at least one filament 150 can circumferentially constrict the elongate member 132 to collapse and seal the elongate member 132 when the constricting mechanism 141 is in the first configuration. The filament can be made from a variety of materials including, for example, a polymer, a synthetic, and/or a metal. In some embodiments, the filament 150 can be nylon, stainless steel, nitinol, silicone, or the like. In some embodiments, the filament can comprise a single strand such as, for example, a monofilament, and in some embodiments, the filament can comprise a plurality of strands that can be, for example, twisted, woven, grouped, and/or fused to form the filament. In some embodiments, the filament 150 can comprise one or several threads, lines, cords, rope, ribbon, flat wire, sheet, or tape.

The filament 150 can be coupled to the actuator 142 such that the filament 150 selectively constricts, collapses, and/or seals the elongate member 132, and specifically the central lumen 138 of the elongate member 132 based on the movement and/or position of the actuator 142. In some embodiments, the filament 150 can be connected to one or both of the buttons 144-A, 144-B such that the filament 150 collapses, constricts, and/or seals the elongate member 132 and specifically the central lumen 138 of the elongate member 132 when the buttons 144-A, 144-B are in the first position, and the filament 150 can be connected to one or both of the buttons 144-A, 144-B such that the elongate member 132 and specifically the central lumen 138 of the elongate member 132 is open and uncollapsed when the buttons 144-A, 144-B are in the second position. In some

embodiments in which the actuator 142 comprises a single button 144, as depicted in FIG. 5, the filament 150 can be connected to the button 144 and to the housing 128 such that the filament 150 is tightened when the button 144 moves to the first position.

In some embodiments, the at least one filament 150 can extend along an axis 152 that can be perpendicular to a central axis 154 of the elongate member 132 and/or of the apertures 124, 126. In some embodiments, the axis 152 of the at least one filament 150 can intersect and be perpendicular to the central axis 154 of the elongate member 132 and/or of the apertures 124, 126. In some embodiments, the actuator 142, and specifically the buttons 144-A, 144-B can move along this axis 152 when moved from the first position to the second position.

In FIG. 3, an embodiment of the valve 104 with the constricting mechanism 141 in the second configuration is shown. As specifically shown, both of the first and second buttons 144-A, 144-B are in the second position, depressed into the retention features 140 of the housing 128. In this second position, the filament 150 is loosened, thereby allowing the expansion of the elongate member 132 and the unsealing of the central lumen 138 of the elongate member 132.

As further seen in FIG. 3, the proximal cap 116 has a proximal end 300 and a distal end 302. The proximal cap 116 can include a funnel portion 301 of the proximal aperture 124, which funnel portion 301 can facilitate insertion of a tool into the proximal aperture 124. The distal end 302 of the proximal cap 116 can partially extend into the interior channel 130 of the housing 128. The proximal cap 116 can include a mating feature 304 that can mate with the proximal

end 134 of the elongate member 132. In some embodiments, the proximal end 134 of the elongate member 132 can fit over the mating feature 304 of the proximal cap 116. The proximal end 134 of the elongate member 132 can be compressed between the mating feature 304 of the elongate member 132 and a portion of the interior channel 130 of the housing 128 into which the mating feature 304 is inserted to thereby secure the proximal end 134 of the elongate member 132 on the mating feature 304. In some embodiments, the proximal end 134 of the elongate member 132 can be further secured on the mating feature 304 by a proximal O-ring 306 that can be compressed between the housing 128 and the mating feature 304 of the proximal cap 116 to sealingly couple the elongate member 132 to the proximal cap 116.

The distal cap 120 has a proximal end 308 and a distal end 310. The distal cap can include a mating feature 312 located on the proximal end 308 of the distal cap 120, which mating feature 312 can mate with the distal end 136 of the elongate member 132. In some embodiments, the distal end 136 of the elongate member 132 can fit over the mating feature 312 of the distal cap 123. The distal end 136 of the elongate member 132 can be compressed between the mating feature 312 of the elongate member 132 and a portion of the interior channel 130 of the housing 128 into which the mating feature 312 is inserted to thereby secure the distal end 136 of the elongate member 132 on the mating feature 312. In some embodiments, the distal end 136 of the elongate member 132 can be further secured on the mating feature 312 by a distal O-ring 314 that can be compressed between the housing 128 and the mating feature 312 of the proximal cap 116 to sealingly couple the elongate member 132 to the distal cap 120.

The distal cap 120 can, in some embodiments, further include a side port barb 314 that can extend laterally away from the distal cap 120 and specifically away from the distal aperture 126 of the distal cap 120. The side port barb 314 can define a side port channel 316 that can extend through the side port barb 314 and fluidly connect to the distal aperture 126. In some embodiments, the side port barb 314 can include a securement feature 318 such as a barb that can secure coupling of a hose or tube to the side port barb 314.

In some embodiments, the side barb 314 can be used to apply a vacuum to the portions of the delivery device 100, and particularly to portions of the delivery device 100 that are distal of the axis 152 along which the elongate member 132 seals. This vacuum can be applied to aspirate a material through the delivery device 100, and specifically through the catheter 102 of the delivery device. This aspirated material can be a biological material including, for example, bodily fluids, multi-phase bodily materials that can include, for example, a fluidic portion and at least one solid portion, or the like.

In some embodiments, due to the narrowing shape of the elongate member 132 when the constricting mechanism 141 is in the first configuration, a vacuum applied to the portions of the delivery device 100 distal to the axis 152 draws the elongate member 132 towards the first configuration and can, in some embodiments, increase the strength, robustness, and/or strength of the seal of the valve 104. This attribute of the valve 104 can provide benefits over other valve designs in which a vacuum can compromise the seal of the valve, and thus the ability to draw a vacuum and aspirate can be limited.

In some embodiments, the valve 104 can further include a reinforcement structure 320 that can extend along all or portions of the elongate member 132. The reinforcement structure 320 can facilitate the uniform collapse of the

11

elongate member 132, can prevent the at least one filament 150 from cutting through and/or tearing the elongate member 132, and can assist in guiding one or several tools through the elongate member 132. The reinforcement structure 320 can be tubular, can extend along and around the elongate member 132, and can be positioned so as to be between the elongate member 132 and the at least one filament 150.

The reinforcement structure 320 can include a proximal end 322 and a distal end 324. In some embodiments, the reinforcement structure 320 extends along and around the elongate member 132, and is positioned such that the proximal end 322 of the reinforcement structure 320 is proximate to the first end 134 of the elongate member 132 and the distal end 324 of the reinforcement structure 320 is proximate to the second end 136 of the elongate member 132.

The reinforcement structure 320 can be coupled to the elongate member 132. In some embodiments, the reinforcement structure 320 is coupled to the elongate member 132 along the length of the reinforcement structure 320, and in some embodiments, the reinforcement structure 320 is coupled to the elongate member 132 and distinct positions along the length of the elongate member 132 and/or the reinforcement structure 320. In one embodiment, for example, the reinforcement structure 320 can be coupled to the elongate member 132 at one or both of the proximal end 322 of the reinforcement structure 320 and the distal end 324 of the reinforcement structure 320 and/or at one or both of the first end 134 and the second end 136 of the elongate member 132. In some embodiments, the reinforcement structure 320 can be coupled to the elongate member 132 via one or several other components of the valve 104. In some embodiments, the reinforcement structure 320 can be coupled to the elongate member 132 via the compression of the reinforcement structure 320 and the elongate member 132 between the housing 128 and one or both of the proximal 116 and the distal 120.

In some embodiments, the reinforcement structure 320 can be adhered to the elongate member 132 via, for example, an adhesive such as silicone adhesive. In some embodiments, the adhesive can be circumferentially applied to the reinforcement structure 320 and/or the elongate member 132 in an adhesive ring that can, for example, have a length approximately between: 0.010 inches and 0.5 inches; 0.02 and 0.4 inches; 0.050 inches and 0.0250 inches, or any other or intermediate range.

In one embodiment, each of the proximal end 322 and the distal end 324 of the reinforcement structure 320 can be adhered via an adhesive to the elongate member 132. In such an embodiment, the reinforcement structure 320 may be uncoupled to the elongate member 132 at positions other than the coupling at one or both of the proximal end 322 and the distal end 324 of the reinforcement structure 320, and thus the reinforcement structure 320 is uncoupled to the elongate member 132 at a position between the first end 134 and the second end 136 of the elongate member 134 and/or between the proximal end 322 and the distal end 324 of the reinforcement structure 320.

The lack of coupling of the reinforcement structure 320 to the elongate member 132 can facilitate and improve the collapse of the elongate member 132 around a tool 400, also referred to herein as instrument 400 or device 400, inserted through the valve 104 as shown in FIG. 4. The tool 400 can be any device inserted through the valve 104 including, for example, one or several additional catheters, lines, wires, grippers, punches, cutters, or the like. As seen in FIG. 4, the

12

tool 400 is inserted through the valve 104 and specifically through the elongate member 132 of the valve. As shown, the constricting mechanism 141 is in the first configuration and the elongate member 132 and the central lumen 138 of the elongate member 132 is collapsed around the tool 400, and specifically around a shaft 402 of the tool 400 to thereby seal the valve 104 around the tool 400 and specifically around the shaft 402 of the tool 400. The constricting mechanism 141 can seal around tools 400 that fit through the elongate member 132, regardless of the size of the tool 400. Thus, the valve can be used with a wide variety of tools. More specifically, the at least one filament 150 can include (i) a first portion 491 extending around at least a portion of the elongate member 132 and (ii) a second portion 492 having a first end 493-A extending from the first portion 491 in one direction and a second end 493-B extending from the first portion 491 in another direction. The first button 144-A can be coupled to the first end 493-A of the at least one filament 150 and the second button 144-B can be coupled to the second end 493-B of the at least one filament 150. In the illustrated first configuration, the at least one filament 150 circumferentially constricts the elongate member 132 to create a seal between the elongate member 132 and the tool 400. The buttons 144-A, 144-B are moveable to the second configuration wherein the at least one filament 150 is moved to at least partially open the central lumen 138 of the elongate member 132.

The reinforcement structure 320 can comprise a variety of designs, shapes, sizes, and materials. In some embodiments, the reinforcement structure 320 can be sized and shaped so as to receive elongate member 132 and to be positioned between the elongate member 132 and the at least one filament 150. In some embodiments, the reinforcement structure 320 can be made from a material sufficiently strong to prevent the cutting of the at least one filament 150 through the elongate member 132.

In some embodiments, the reinforcement structure can comprise a coil or a mesh sheath. The mesh sheath can, in some embodiments, comprise a braided mesh. The braided mesh can be made from any desired number of wires in any desired configuration. In some embodiments, the braided mesh can comprise a 4 wire braided mesh, an 8 wire braided mesh, a 12 wire braided mesh, a 16 wire braided mesh, a 20 wire braided mesh, a 24 wire braided mesh, a 32 wire braided mesh, a 48 wire braided mesh, a 64 wire braided mesh, a 72 wire braided mesh, an 80 wire braided mesh, a 96 wire braided mesh, or any other or intermediate braided mesh. In some embodiments, the braided mesh can comprise: a 1x1 configuration. In some embodiments, the wire in the braided mesh can be any desired material including, for example, a metal wire such as a nitinol wire or a stainless steel wire, a polymer wire, or a natural wire. In one embodiment, the braided mesh can comprise a 48 wire mesh in a 1x1 configuration made with a nitinol wire having a diameter of 0.003 inches.

With reference now to FIGS. 6 through 9, different embodiments and/or configurations of the filament 150 are shown. The filament 150 can comprise a single filament 150 having a first end 600 and a second end 602 as shown in FIG. 6. The filament 150, and specifically which first and second ends 600, 602 can be coupled to the actuator 142 to move the filament 150 between the first and second configurations or positions and/or from the first configuration or position to the second configuration or position. In some embodiments, both of the first end 600 and the second end 602 can be coupled to a single button 144, in some embodiments, each of the first end 600 and the second end 602 can be coupled

13

to different buttons **144**, and in some embodiments, one of the first end **600** and the second end **602** can be coupled to a button **144** and the other of the first end **600** and the second end **602** can be coupled to the housing **128** or other portion of the valve **104**.

In some embodiments, the filament **150** can comprise multiple filaments, and specifically, as shown in FIGS. **7** through **9**, the filament **150** can comprise a first filament **150-A** and a second filament **150-B**. In embodiments in which the filament **150** comprises multiple filaments, each of the multiple filaments can have a first end **700** and a second end **702**. The first and second filaments **150-A**, **150-B** can be coupled to the actuator **142**. In such embodiments, the first and second ends **700**, **702** can be coupled to the actuator **142** to move the filaments **150-A**, **150-B** between the first and second configurations and/or from the first configuration to the second configuration. In some embodiments, both of the first end **700** and the second end **702** of one or more of the multiple filaments **150** can be coupled to a single button **144**, in some embodiments, each of the first end **700** and the second end **702** of one or more of the multiple filaments **150** can be coupled to different buttons **144**, and in some embodiments, one of the first end **700** and the second end **702** of one or more of the multiple filaments **150** can be coupled to one button **144** and the other of the first end **700** and the second end **702** of those one or more filaments **150** can be coupled to the housing **128** or other portion of the valve **104**.

The filament **150** can be arranged in a variety of configurations. In some embodiments, the filament **150** can be configured to form a single loop **604** that can extend around the elongate member **132** and/or through which the elongate member **132** can be received as shown in FIG. **6**, and in some embodiments, the filament **150** can be configured to form multiple loops, and specifically a first loop **704** and a second loop **706** as shown in FIG. **7**. The first and second loops **704**, **706** can each receive the elongate member **132**. In some embodiments, a diameter or size of the loop **604**, or of the loops **704**, **706** can decrease when the constricting mechanism **141** is moved from the second configuration to the first configuration.

In some embodiments, the filament **150** can be configured to form a bight **800**, which bight **800** can be a single bight or multiple bights. As used herein, a “bight” refers to a U-shaped section between the two ends of the filament **150**. As depicted in FIGS. **8** and **9**, the bight **800** can comprise multiple bights, and specifically a first bight **800-A** and a second bight **800-B**. In some embodiments, the first bight **800-A** can extend through the second bight **800-B** such that the first and second bights **800-A**, **800-B** interlock, whereas in other embodiments, the first and second bights **800-A**, **800-B** can be non-interlocking. Similarly, in embodiments containing the filament **150** having multiple loops, one or several of the multiple loops can be interlocking.

In some embodiments, the bight **800**, and specifically one or both of the first bight **800-A** and the second bight **800-B** can be formed around a portion of the elongate member **132** and/or can extend around a portion of the elongate member **132**. Each bight **800** can define a partially enclosed receiving area **808** wherein the elongate member **132** can be received. Thus, the first bight **800-A** can define a first receiving area **808-A** and the second bight **800-B** can define a second receiving area **808-B**.

As seen in FIGS. **8** and **9**, multiple bights, and specifically the first and the second bights **800-A**, **800-B** can be positioned and oriented such that the first bight **800-A** has a first orientation or first direction as indicated by arrow **810**, and

14

the second bight has a second orientation or second direction as indicated by the arrow **812**. In some embodiments, the first orientation is different from the second orientation such that the first and second receiving areas **808-A**, **808-B** overlap and define an encircled area **814**, also referred to herein as a constricting area **814**. The elongate member **132** can be received within the encircled area **814**. In embodiments in which bights **800-A**, **800-B** overlap to define the encircled area **814**, the movement of the constricting mechanism **141** to the first configuration can result in and/or include the first bight **800-A** moving in the direction indicated by the arrow **810** and/or the second bight **800-B** moving in the direction indicated by the arrow **812**, which movement of the bights **800-A**, **800-B** decreases the size of the encircled area **814** and constricts, collapses, and/or seals the elongate member **132** extending through the encircled area **814**.

The filament(s) **150** forming the bights **800** can each apply an arcuate line or narrow longitudinal zone of pressure to the elongate member **132**. If the filament(s) are circular in cross-section, the zone of pressure can be very small, and can, in some embodiments, be less than the diameter or thickness of the filament. In some embodiments, the filaments have a diameter or width less than about 2.5 mm, less than about 2 mm, less than about 1.5 mm, less than about 1.25 mm, less than about 1 mm, less than about 0.75 mm, less than about 0.5 mm, and/or less than about 0.25 mm. In some embodiments, the filaments can have a diameter or width of between about 0.01 mm and 2.5 mm, between about 0.05 mm and 2 mm, between about 0.1 mm and 1 mm, and/or between about 0.125 mm and 0.70 mm. In some embodiments, the arcuate line or zone of pressure may form two opposing arcs and in other embodiments, the arcuate line of pressure may be a singular substantially circular line or zone that encircles the elongate member at least once. The longitudinal length of the of the line or zone of pressure may be very short compared to other valves known in the art. In some embodiments, the longitudinal length of the zone of pressure applied to the elongate member **132** by the filament (s) **150** may be less than about 2.0 mm and in some embodiments less than about 0.5 mm. In some embodiments, the filament(s) **150** can have any desired cross-sectional shape including, for example, a circular cross-section, a rectangular cross-section, an oval cross-section, a square cross-section, a polygonal cross-section, a triangular cross-section, or any other desired shape of cross-section.

With reference now to FIG. **10**, a flowchart illustrating one embodiment of a process **1000** for sealing a valve **104** and/or catheter **102** accessing a body of a patient is shown. The process **1000** can be performed using the valve **104** and/or the delivery system **100**. The process **1000** begins at block **1002**, wherein the delivery device **100**, and specifically the catheter **102** of the delivery device **100** is inserted into the body of the patient. In some embodiments, this can include inserting the catheter **102** into a portion of the circulator system of the patient such as, for example, a blood vessel including an artery or a venous vessel. In some embodiments, the delivery device **100** can be inserted into the body of the patient directly through an aperture or incision in the patient, and in some embodiments, the delivery device **100** can be inserted into the body of the patient via another catheter or device. In some embodiments, the constricting mechanism **141** can be in the first configuration while the delivery device **100** and/or the catheter **102** is inserted into the patient’s body.

After the delivery device **100** is inserted into the body of the patient, the process **1000** proceeds to block **1004**,

15

wherein the constricting mechanism **141** is moved from the first configuration to the second configuration. As described above, the central lumen **138** of the elongate member **132** is unsealed when the constricting mechanism **141** is in the second configuration. In some embodiments, the moving of the constricting mechanism **141** from the first configuration to the second configuration can include the manipulation of the actuator **142** and/or the control of the actuator **142**, and specifically the depressing of the one or several buttons **144** to move the filament **150** from the first position to the second position to allow the expansion and opening of the central lumen **138** of the elongate member **132**.

After the constricting mechanism **141** is moved from the first configuration to the second configuration, the process **1000** proceeds to block **1006**, wherein the tool **400**, and specifically the shaft **402** of the tool **400** is advanced through the delivery device **100** and specifically through the valve **104** until a first end of the tool reaches a desired position within the body of the patient. In some embodiments, a portion of the shaft **402** can be positioned within the central lumen **138** of the elongate member **132** after the advancing of the tool **400** through the delivery device **100**. In some embodiments, after the tool **400** is advanced through the delivery device **100**, the desired procedure can be performed with the tool.

After the tool **400** is advanced through the delivery device **100**, or while the tool **400** is being advanced through the delivery device **100**, the process **1000** proceeds to block **1008**, wherein the constricting mechanism **141** is returned to the first configuration. In some embodiments, the returning of the constricting mechanism **141** to the first configuration can include the release of the one or several buttons **144** and/or the control of the actuator **142** to reconfigure the constricting mechanism **141** to the first configuration. In some embodiments, the return of the constricting mechanism **141** to the first configuration can result in the collapse and/or sealing of the elongate member **132** and specifically the central lumen **138** of the elongate member **132** around the tool **400** and specifically around the shaft **402** of the tool **400**. The return of the constricting mechanism **141** to the first configuration, or the movement of the constricting mechanism **141** to the first configuration can include the decreasing of the size and/or diameter of one or several loops formed by the filament **150** and/or the movement of one or several bights **800** such as, for example, the movement of the first bight **800-A** in the first direction indicated by arrow **810** and the movement of the second bight **800-B** in the second direction indicated by arrow **812** to reduce the size of the constricting area **814**. In some embodiments, after the constricting mechanism is returned to the first configuration, the desired procedure can be performed with the tool.

After the constricting mechanism is returned to the first configuration, the process **1000** proceeds to block **1010**, wherein the tool **400**, and specifically the shaft **402** of the tool **400** is retracted from the delivery device **100**, and more specifically from the valve **104**. In some embodiments, the valve **104** can remain sealed during the retracting of the tool **400** and/or the shaft **402** of the tool. In some embodiments, the valve **104** remains sealed during the retracting of the tool **400** and/or the retracting of the shaft **402** of the tool **400** as the constricting mechanism **141** can remain in the first configuration during the retracting of the tool **400** and/or the shaft **402** of the tool **400**.

In some embodiments, the constricting mechanism **141** can be moved to the second configuration to allow the retraction of the tool **400** and/or the shaft **402** of the tool **400** from the valve **104**, and the constricting mechanism **141** can

16

be returned to the first configuration when the tool **400** and/or the shaft **402** of the tool **400** is removed from the valve **104**. In some embodiments, the retraction of the tool **400** and/or shaft **402** of the tool **400** from the valve **104** can be performed with the constricting mechanism **141** left in the first configuration. In some embodiments, the constricting mechanism **141** can be moved to the second configuration, and then returned to the first configuration via the manipulation and/or control of the actuator **142**, which manipulation and/or control of the actuator **142** can include the depressing of the one or several buttons **144** to move the constricting mechanism **141** to the second configuration, and the release of the one or several buttons **144** to return the constricting mechanism **141** to the first configuration. In some embodiments, if the procedure is complete, the delivery device **100** can then be removed from the body of the patient, and any incision created for the procedure can be closed.

With reference now to FIG. **11**, a side view of one embodiment of a thrombectomy system **1100** including the delivery device **100** and a thrombus extraction device **1102** is shown. In some embodiments, the thrombectomy system **1100** can be used to access a blood vessel **1104** to treat and/or extract a thrombus **1106** from the blood vessel **1104**. The thrombus extraction device **1102** can include a self-expanding coring element **206** and expandable cylindrical portion **208**. In some embodiments, and as shown in FIG. **11**, the thrombus extraction device **1102** can be the tool **400** that can extend through the valve **104**, and in some embodiments, the valve **104** can be a part of the thrombus extraction device **1102**. Further details of thrombectomy systems, thrombus extraction devices, and methods of using the same are disclosed in: U.S. application Ser. No. 15/268,296, filed Sep. 16, 2016, and entitled "INTRAVASCULAR TREATMENT OF VASCULAR OCCLUSION AND ASSOCIATED DEVICES, SYSTEMS, AND METHODS"; U.S. application Ser. No. 15/498,320, filed Apr. 26, 2017, and entitled "DEVICES AND METHODS FOR TREATING VASCULAR OCCLUSION"; and U.S. application Ser. No. 15/466,740, filed on Mar. 22, 2017, and entitled "DEVICE AND METHOD FOR TREATING VASCULAR OCCLUSION", the entirety of each of which is hereby incorporated by reference herein.

With reference now to FIG. **12**, a side-section view of another embodiment of the hemostasis valve **104** having two piece caps **116**, **120** is shown. The valve **104** can include a housing **128** defining an interior channel **130** through which the tubular member **132** can extend. The valve **104** can include the proximal cap **116** and the distal cap **120**. In some embodiments, the proximal cap **116** can comprise a two piece cap and can include a proximal exterior member **1200** and a proximal channel member **1202**. In some embodiments, the distal cap **120** can comprise a two-piece cap and can include a distal exterior member **1204** and a distal channel member **1206**. In some embodiments, this coupling between the proximal exterior member **1200** and the proximal channel member **1202** and/or the coupling between the distal exterior member **1204** and the distal channel member **1206** can be a sealed coupling so as to prevent the leakage of material including fluid or gas between the respective ones of the proximal exterior member **1200** and the proximal channel member **1202** and/or the distal exterior member **1204** and the distal channel member **1206**. In some embodiments, this sealing coupling can be achieved and/or maintained via a seal such as an O-ring **1208** that can be positioned between the proximal exterior member **1200** and

17

the proximal channel member **1202** and/or between the distal exterior member **1204** and the distal channel member **1206**.

In some embodiments, the proximal exterior member **1200** can be coupled, and in some embodiments, rotatably coupled to the proximal channel member **1202** in a manner to allow the rotation of the proximal exterior member **1200** without rotating the proximal channel member **1202**. Similarly, in some embodiments, the distal exterior member **1204** can be rotatably coupled to the distal channel member **1206** in a manner to allow the rotation of the distal exterior member **1204** without the rotating of the distal channel member **1206**. In some such embodiments, the channel members **1202**, **1206** can be non-rotatable with respect to the housing **128** and/or the tubular member **132**, and one or both of the exterior members **1200**, **1204** can be rotatable with respect to the housing **128** and/or the tubular member **132**. In such an embodiment, the maintaining of the rotational position of the channel members **1202**, **1206** with respect to the housing **128** and/or the tubular member **132** can prevent the twisting of the tubular member **132** which can result in the sealing of the tubular member **132** regardless of the configuration of the constructing mechanism **141**.

The exterior members **1200**, **1204** can comprise a variety of shapes and sizes and can include a variety of features. In some embodiments, one or both of the exterior members **1200**, **1204** can be coupled to, for example, a shaft similar to the shaft **106** shown in FIG. 1. In some embodiments, for example, the distal exterior member **1204** can be coupled to a shaft **106**, including, for example, can be non-detachably coupled to the shaft **106**. In some embodiments, one or both of the exterior members can include one or several features configured to facilitate coupling with the valve **104**. These one or several features can include, for example, one or several male or female: connectors; couplers; attachment mechanisms; or the like. In some embodiments, these one or several features can facilitate use of the valve with other existing components, instruments, tools, or the like. In some embodiments, for example, one or both of the exterior members **1200**, **1204** can comprise either a male or female luer fitting, and specifically as shown in FIG. 12, the distal exterior member **1204** can comprise a male luer fitting **1210**.

Several aspects of the present technology are set forth in the following examples.

1. A hemostatic valve for sealing a medical device, the hemostatic valve comprising:

an elongate member having a first end, a second end, and a central lumen extending therebetween, wherein the elongate member is pliable;

a reinforcement structure extending along at least a portion of the elongate member, wherein the reinforcement structure is coupled to the elongate member; and

an active tensioning mechanism coupled to the elongate member, wherein the tensioning mechanism is moveable between a first configuration wherein the central lumen is constricted and sealed and a second configuration wherein the central lumen is open.

2. The hemostatic valve of example 1, wherein the elongate member comprises a compliant polymer tube.

3. The hemostatic valve of example 1 or 2, wherein the tensioning mechanism comprises at least one filament extending at least partially around the elongate member.

4. The hemostatic valve of example 3, wherein the reinforcement structure is positioned between the at least one filament and the elongate member.

5. The hemostatic valve of example 4, wherein the reinforcement structure comprises a braided mesh.

18

6. The hemostatic valve of example 4 or 5, wherein the reinforcement structure is coupled to the elongate member at a position proximate to the first end of the elongate member and at a position proximate to the second end of the elongate member.

7. The hemostatic valve of example 6, wherein the reinforcement structure is not coupled to the elongate member at a position between the first end of the elongate member and the second end of the elongate member.

8. The hemostatic valve of any one of examples 3-7, wherein the tensioning mechanism comprises an actuator coupled to the at least one filament, wherein the actuator is moveable to control movement of the at least one filament from a first position wherein the central lumen is constricted and sealed to a second position wherein the central lumen is open, wherein the at least one filament is in the first position when the tensioning mechanism is in the first configuration.

9. The hemostatic valve of example 8, wherein the actuator is biased towards the first position.

10. The hemostatic valve of example 8 or 9, wherein the actuator is biased toward the second position.

11. The hemostatic valve of any one of examples 8-10, wherein the actuator comprises a manual actuator.

12. The hemostatic valve of any one of examples 8-11, wherein the at least one filament forms a loop around the elongate member.

13. The hemostatic valve of any one of examples 8-12, wherein the at least one filament forms a bight around a portion of the elongate member.

14. The hemostatic valve of any one of examples 8-13, wherein the at least one filament comprises a first filament and a second filament, wherein each of the first filament and the second filament are coupled to the actuator, and wherein the first filament and the second filament are moveable from the first position to the second position.

15. The hemostatic valve of example 14, wherein each of the first filament and the second filament form a loop around the elongate member.

16. The hemostatic valve of example 14 or 15, wherein the first filament forms a first bight around a first portion of the elongate member, and wherein the second filament forms a second bight around a second portion of the elongate member.

17. The hemostatic valve of example 16, wherein the first bight extends through the second bight.

18. The hemostatic valve of any one of examples 1-17, further comprising a shell defining a first aperture and a second aperture, wherein the elongate member extends from the first aperture to the second aperture and fluidly couples the first aperture and the second aperture.

19. The hemostatic valve of any one of examples 1-18, wherein the tensioning mechanism is self-adjustable to seal around tools of different sizes extending through the hemostatic valve.

20. The hemostatic valve of any one of examples 1-19, wherein the central lumen comprises a single lumen.

21. The hemostatic valve of any one of examples 1-20, wherein the central lumen comprises a plurality of lumens.

22. A delivery system for intravascular access of a blood vessel within a patient's body, the delivery system comprising:

a catheter having a first end, a second end, and a catheter lumen extending therebetween;

a hemostatic valve coupled to the first end of the catheter, the hemostatic valve comprising:

a tubular member having a first end, a second end, and a central lumen extending therebetween, wherein the

19

central lumen of the tubular member is fluidly coupled with the catheter lumen; and
 an active tensioning mechanism coupled to the tubular member, the tensioning mechanism moveable between a first configuration wherein the tensioning mechanism constricts on the central lumen and the central lumen is sealed and a second configuration wherein the central lumen is open.

23. The delivery system of example 22, wherein the hemostatic valve further comprises a reinforcement structure extending along at least a portion of the tubular member.

24. The delivery system of example 22 or 23, wherein the reinforcement structure is located between the tensioning mechanism and the tubular member.

25. The delivery system of example 24, wherein the reinforcement structure comprises a braided mesh.

26. The delivery system of example 24 or 25, wherein the reinforcement structure is coupled to the tubular member at a position proximate to the first end of the tubular member and at a position proximate to the second end of the tubular member.

27. The delivery system of example 26, wherein the reinforcement structure is adhered to the tubular member at the first end of the tubular member and at the second end of the tubular member.

28. The delivery system of example 27, wherein the reinforcement structure is uncoupled to the tubular member between the first end of the tubular member and the second end of the tubular member.

29. The delivery system of any one of examples 22-28, wherein the tensioning mechanism comprises at least one filament extending at least partially around the tubular member.

30. The delivery system of example 29, wherein the tensioning mechanism comprises an actuator coupled to the at least one filament, wherein moving the tensioning mechanism from the first configuration to the second configuration comprises moving the actuator and the thereto coupled at least one filament from a first position to a second position, wherein the filament constricts and seals the central lumen of the tubular member when the filament is in the first position.

31. The delivery system of example 30, wherein the actuator comprises a manual actuator.

32. The delivery system of example 31, wherein the actuator comprises a pair of opposing and depressable buttons, wherein the buttons are biased towards an undepressed position.

33. The delivery system of example 31 or 32, wherein the central lumen is sealed when the buttons are in the undepressed position.

34. The delivery system of any one of examples 30-33, wherein the filament comprises a monofilament.

35. The delivery system of any one of examples 30-34, wherein the filament comprises at least one of: a polymer filament; or a metallic filament.

36. The delivery system of any one of examples 22-35, wherein the catheter comprises a thrombus extraction device.

37. A method of sealing a delivery device accessing a blood vessel of a patient, the method comprising:

inserting the delivery device comprising a catheter and a hemostatic valve into the blood vessel of the patient, the catheter having a first end, a second end, and a catheter lumen extending therethrough, and the hemostatic valve coupled to the first end and having a tubular member defining a central lumen fluidly coupled with

20

the catheter lumen and a tensioning mechanism coupled with the tubular member, wherein the tensioning mechanism collapses and seals the central lumen in a first configuration and thereby seals access to the blood vessel;

moving the tensioning mechanism of the hemostatic valve to a second configuration, wherein the central lumen is open and access to the blood vessel is unsealed when the tensioning mechanism is in the second configuration;

advancing a shaft of a tool through the delivery device until a first end of the tool reaches a desired position within the blood vessel of the patient and a portion of the shaft is positioned within the central lumen of the tubular member; and

returning the tensioning mechanism of the hemostatic valve to the first configuration such that the tubular member collapses on the shaft of the tool and seals around the shaft of the tool.

38. The method of example 37, further comprising retracting the shaft of the tool from the delivery device.

39. The method of example 38, wherein the tensioning mechanism is maintained in the first configuration during and after the retracting of the shaft of the tool from the delivery device.

40. The method of example 38 or 39, wherein the tensioning mechanism is moved to the second configuration during the retracting of the shaft of the tool from the delivery device, and wherein the tensioning mechanism is returned to the first configuration after the shaft of the tool is retracted from the delivery device.

41. The method of any one of examples 37-40, wherein the tensioning mechanism comprises at least one filament extending at least partially around the tubular member, wherein the at least one filament collapses the tubular member when the tensioning mechanism is in the first configuration.

42. The method of example 41, wherein the at least one filament circumferentially constricts the tubular member to collapse the tubular member when the tensioning mechanism is in the first configuration.

43. The method of example 41 or 42, wherein the hemostatic valve comprises a reinforcement structure located between the at least one filament and the tubular member.

44. The method of any one of examples 41-43, wherein the at least one filament forms a loop around the elongate member, and wherein moving the tensioning mechanism from the second configuration to the first configuration reduces a size of the loop to thereby constrict the tubular member within the loop.

45. The method of any one of examples 41-44, wherein the filament forms at least one bight around a portion of the elongate member.

46. The method of example 45, wherein the filament comprises a first filament and a second filament, and wherein the at least one bight comprises a first bight oriented in a first direction and formed by the first filament and a second bight oriented in a second direction and formed by the second filament, wherein the first and second bights overlap to encircle a portion of the tubular member within an constricting area.

47. The method of example 46, wherein moving the tensioning mechanism from the second configuration to the first configuration comprises moving the first bight in the first direction and the second bight in the direction to reduce the size of the constricting area and collapse and seal the central lumen of the tubular member.

21

48. The method of any one of examples 37-47, wherein the tensioning mechanism comprises an actuator, and wherein moving the tensioning mechanism to the second configuration comprises manipulating the actuator.

49. The method of any one of examples 37-48, further comprising applying a vacuum to the delivery device to aspirate material through the catheter, wherein the central lumen remains sealed during the aspiration.

50. The method of any one of examples 37-49, wherein the tool comprises a thrombus extraction device.

51. A hemostatic valve for sealing a medical device, the hemostatic valve comprising:

an elongate member having a first end, a second end, and a central lumen comprising a plurality of lumens extending therebetween, wherein the elongate member is pliable; and

an active tensioning mechanism coupled to the elongate member, wherein the tensioning mechanism is moveable between a first configuration wherein the central lumen is constricted and sealed and a second configuration wherein the central lumen is open.

Other variations are within the spirit of the present invention. Thus, while the invention is susceptible to various modifications and alternative constructions, certain illustrated embodiments thereof are shown in the drawings and have been described above in detail. It should be understood, however, that there is no intention to limit the invention to the specific form or forms disclosed, but on the contrary, the intention is to cover all modifications, alternative constructions, and equivalents falling within the spirit and scope of the invention, as defined in the appended claims.

In the previous description, various embodiments of the present invention are described. For purposes of explanation, specific configurations and details are set forth in order to provide a thorough understanding of the embodiments. However, it will also be apparent to one skilled in the art that the present invention may be practiced without the specific details. Furthermore, well-known features may be omitted or simplified in order not to obscure the embodiment being described.

The use of the terms “a” and “an” and “the” and similar referents in the context of describing the invention (especially in the context of the following claims) are to be construed to cover both the singular and the plural, unless otherwise indicated herein or clearly contradicted by context. The terms “comprising,” “having,” “including,” and “containing” are to be construed as open-ended terms (i.e., meaning “including, but not limited to,”) unless otherwise noted. The term “connected” is to be construed as partly or wholly contained within, attached to, or joined together, even if there is something intervening. Recitation of ranges of values herein are merely intended to serve as a shorthand method of referring individually to each separate value falling within the range, unless otherwise indicated herein, and each separate value is incorporated into the specification as if it were individually recited herein. All methods described herein can be performed in any suitable order unless otherwise indicated herein or otherwise clearly contradicted by context. The use of any and all examples, or exemplary language (e.g., “such as”) provided herein, is intended merely to better illuminate embodiments of the invention and does not pose a limitation on the scope of the invention unless otherwise claimed. No language in the specification should be construed as indicating any non-claimed element as essential to the practice of the invention.

Preferred embodiments of this invention are described herein, including the best mode known to the inventors for

22

carrying out the invention. Variations of those preferred embodiments may become apparent to those of ordinary skill in the art upon reading the foregoing description. The inventors expect skilled artisans to employ such variations as appropriate, and the inventors intend for the invention to be practiced otherwise than as specifically described herein. Accordingly, this invention includes all modifications and equivalents of the subject matter recited in the claims appended hereto as permitted by applicable law. Moreover, any combination of the above-described elements in all possible variations thereof is encompassed by the invention unless otherwise indicated herein or otherwise clearly contradicted by context.

All references, including publications, patent applications, and patents, cited herein are hereby incorporated by reference to the same extent as if each reference were individually and specifically indicated to be incorporated by reference and were set forth in its entirety herein.

The invention claimed is:

1. A valve, comprising:

a tubular member defining a lumen configured to slidably receive a catheter;

a constricting mechanism including at least one filament and an actuator coupled to the filament, the filament comprising a first portion extending around at least a portion of the tubular member and a second portion having a first end extending from the first portion in one direction and a second end extending from the first portion in another direction, and the actuator comprises a first member coupled to the first end of the filament and a second member coupled to the second end of the filament, wherein the first member and the second member of the actuator are moveable between (a) a first position wherein the filament circumferentially constricts the lumen to create a seal and (b) a second position wherein the filament is moved to at least partially open the lumen; and

a biasing system configured to bias the first member and the second member to the first position.

2. The valve of claim 1 wherein the tubular member is pliable.

3. The valve of claim 1 wherein the first portion of the filament extends in a loop completely around the tubular member.

4. The valve of claim 1 wherein the first member of the actuator comprises a first button and the second member of the actuator comprises a second button, wherein the first button and the second button are undepressed in the first position, and wherein the first button and the second button are depressed in the second position.

5. The valve of claim 1 wherein, when the first member and the second member of the actuator are in the first position, the lumen of the tubular member is configured to remain constricted and sealed when a pressure differential exists between (a) a first volume outside the lumen and adjacent to a first end of the tubular member and (b) a second volume outside the central lumen and adjacent to a second end of the tubular member.

6. The valve of claim 1 wherein, when the first member and the second member of the actuator are in the first position, the lumen of the tubular member is configured to remain constricted and sealed when vacuum pressure is applied to a volume outside the lumen and adjacent to either a first end or a second end of the tubular member.

7. The valve of claim 1 wherein the lumen of the tubular member extends a long a first longitudinal axis, wherein the first member and the second member of the actuator are

movable between the first and second positions along a second longitudinal axis, and wherein the first longitudinal axis is orthogonal to the second longitudinal axis.

8. The valve of claim 1 wherein the biasing system comprises a first compression spring coupled to the first member and a second compression spring coupled to the second member. 5

9. The valve of claim 1 wherein, in the first position, the first member and the second member of the actuator pull the filament to circumferentially constrict the tubular member such that the lumen is constricted and sealed. 10

* * * * *